Ceyear 思仪

87235 Series
USB Average Power Sensor
Programming Manual



Ceyear Technologies Co., Ltd.

This Manual applies to the following models of USB Average Power Sensor based on the firmware version of 1.0 and higher.

- 87235B Average Power Sensor, frequence range: 8kHz~8GHz, power range: -70dBm~+26dBm
- 87235C Average Power Sensor, frequence range: 10MHz~8GHz, power range: -60dBm~+23dBm
- 87235D Average Power Sensor, frequence range: 10MHz~18GHz, power range: -70dBm~+26dBm
- 87235F Average Power Sensor, frequence range: 10MHz~33GHz, power range: -65dBm~+26dBm
- 87235FA Average Power Sensor, frequence range: 10MHz~40GHz, power range: -65dBm~+23dBm
- 87235H Average Power Sensor, frequence range: 10MHz~50GHz, power range: -65dBm~+23dBm

Version: B.2 March, 2025, Ceyear Technologies Co., Ltd.

Address: No. 98, Xiangjiang Road, Huangdao District, Qingdao City, Shandong Province
Service Inquires: 400-1684191
Quality supervision: 0532-86886614
Website: www.ceyear.com
E-mail: techbb@ceyear.com
Zip code: 266555

Foreword

Thank you for choosing and using the 87235 series average power sensor developed and produced by Ceyear Technologies Co., Ltd.! Integrating high, sophisticated and cutting-edge technologies, our products offer high cost performance among similar products.

We will take the responsibility to maximally meet your needs and provide you with high-quality measuring instruments and first-class after-sales service. We aim to provide "high quality and considerate service", and operate on the principle of making customers satisfactory with our products and services.

Manual No.

AV2.984.1545SCEN

Version

B.2 2025.03

Ceyear Technologies Co., Ltd.

Manual Authorization

The contents of this manual are subject to change without notice. The contents and terms used in this manual are interpreted by Ceyear Technologies Co., Ltd.

The copyright of the manual belongs to Ceyear Technologies Co., Ltd, no modification can be made to the manual contents by any unit or person without approval of the Company, and no reproduction or propagation of the manual can be made for profits, otherwise, Ceyear Technologies Co., Ltd reserves the right of pursuing legal responsibilities from any infringer.

Product warranty

The warranty period of this product is 18 months from the date of shipment. The instrument manufacturer will repair or replace the damaged components according to the user's requirements and actual conditions within the warranty period. For specific maintenance issues, see the contract.

Product quality certificate

This product is guaranteed to meet the specifications in this manual from the date of shipment. The calibration and measurement are completed by measuring bodies with national qualification, with relevant data to be provided for reference by users.

Quality/Environmental Management

This product complies with the quality and environmental management systems during R&D, manufacturing and testing. Ceyear Technologies Co., Ltd. is qualified and has passed ISO 9001 and ISO 14001 management systems.

Safety Precautions

NOTICE

The "Notice" symbol indicates some important information which will not cause danger. It reminds the user to pay attention to a certain operation process, operation method or the like. In case of any failure of observing the rule or maloperation, instrument damage or important data loss can occur. Further operation cannot be proceeded until the conditions are fully understood and met operation.

TIPS

The "Tips" symbol indicates information tips. It reminds the user to pay attention to the instrument or certain operation process, operation method or the like. The purpose is to guide the instrument operator to use the instrument correctly.

Contents

1 Manual navigation····· 1
1.1 About the Manual····· 1
1.2 Related Documents····· 2
2 Remote Control····· 3
2.1 Remote Control Basics····· 3
2.1.1 Program Control Interface····· 3
2.1.2 Message····· 7
2.1.3 SCPI····· 8
2.1.4 Command Sequence and Synchronization····· 19
2.1.5 Status Reporting System····· 21
2.1.6 Programming Precautions····· 29
2.2 Instrument Program Port and Configuration····· 29
2.3 I/O library····· 30
2.3.1 Overview of I/O Library····· 30
2.3.2 Installation and Configuration of I/O Library····· 31
2.4 Zeroing····· 31
2.4.1 Internal zeroing····· 32
2.4.2 External zeroing····· 32
2.5 Performing Measurements····· 32
2.6 Using Frequency Response Offset Table····· 32
2.6.1 Overview····· 33
2.6.2 Input Frequency Offset Table····· 33
2.6.3 Select Frequency Offset Table····· 34
2.6.4 Enable Frequency Offset Table····· 34
2.6.5 Measurement Applications····· 34
2.6.6 Specific Applications····· 34
2.7 Setting Display Resolution····· 34

Contents

2.8 Setting Average····· 35
2.8.1 Measurement Average····· 35
2.8.2 Video Average····· 35
2.9 Setting Offset····· 35
2.10 Setting Measurement Limits····· 35
2.11 Status Report····· 36
2.12 Storing/Recalling····· 37
3 Program Control Commands····· 39
3.1 Description of Commands····· 39
3.2 General Commands(IEEE488.2 Commands)····· 39
3.3 Instrument Subsystem Command····· 46
3.3.1 Calculation Subsystem Command (CALCulate)····· 46
3.3.2Calibration Sub-system Command (CALibration)····· 55
3.3.3 Measurement Subsystem Command (CONFigure/FETCh/READ/MEASure)·· 56
3.3.4 Display Subsystem Command (DISPlay)····· 65
3.3.5 Format Subsystem Command (FORMat)····· 66
3.3.6 Memory Subsystem Command (MEMory/MMEMory)····· 67
3.3.7 Sensor Subsystem Command (SENSe)····· 73
3.3.8 Status Subsystem Command (STATus)····· 89
3.3.9 System Subsystem Command (SYSTem)····· 128
3.3.10 Trigger Subsystem Command (INITiate/ TRIGger)····· 143
3.3.11 Unit Subsystem Command (UNIT)····· 150
3.3.12 Service Subsystem Command (SERVice)····· 151
4 Programming Examples····· 155
4.1 Basic Operation Examples····· 155
4.1.1 VISA Library····· 155
4.1.2 Example Runtime Environment····· 156
4.1.3 Initialize and Set Default State····· 157

4.1.4 Send Setting Command····· 158
4.1.5 Read the State of Measuring Instrument·····158
4.1.6 Command Synchronization·····159
4.2 Advanced Operation Examples····· 160
4.2.1 USBTMC Program Control Example····· 160
4.2.2 Linux development examples·····164
4.3 Application Examples····· 165
4.3.1 Fast build-up of top-of-pulse average power measurements with "gates” 165
4.3.2 GSM timeslot measurements in list mode····· 165
4.3.3 External Trigger Buffer Measurement·····166
4.3.4 External Trigger Buffer Sweep Measurement·····166
4.3.5 Fast Measurement Mode (Free Run)····· 167
4.3.6 Fast Measurement Mode (External Trigger)····· 167
4.3.7 Continuous and Uninterrupted Measurements·····168
5 Error Description·····171
5.1 Error Message·····171
5.2 Method to Obtain After-sales Services····· 175
5.2.1 Contact us····· 175
5.2.2 Package and mailing····· 176
Appendixes····· 177
Appendix A Zoom Table of SCPI Classified by Subsystem····· 177

1 Manual navigation

This chapter introduces the program control manual functions, chapter structure and main contents of the 87235 series USB average power probe (hereinafter to as the 87235), as well as the instrument-related documents provided to users.

- About the Manual.....1
- Related Documents.....2

1.1 About the Manual

This manual introduces the methods for remote control of the 87235 and application of SCPI. Meanwhile, in order to make it convenient for users to quickly master the remote control programming methods, some programming examples are listed, and the basic concept of I/O function library is introduced. To facilitate your skillful use of such instrument, please read carefully and follow this manual in advance for correct operation.

SCPI (Standard Commands for Programmable Instruments) define the standards and methods for remote control of the instrument, and are the remote control programming language for programmable electronic test and measuring instruments. SCPI are based on the IEEE 488.2 standard and form. Please refer tohttp://www.scpiconsortium.orgfor details.

The manual details the program control command of the 87235.

The chapters of the program control manual include:

- Remote Control

The methods for remote control of the instrument are summarized to make users get familiar with remote control quickly. It is divided into three parts: remote control basics, introducing program related concepts, software configuration, program port, SCPI, etc.; instrument port configuration method, introducing the connection method and software configuration method for program ports of the 87235; I/O function library, introducing the basic concept of instrument driver and basic installation instructions of IVI-COM/IVI-C driver.

- Program Control Commands

Common commands, instrument commands and compatible commands are introduced, and the functions, parameters and examples of SCPI are described.

- Programming Examples

The basic programming examples and advanced programming examples are provided in the way of text description and example code, and the explanation is provided to make it convenient for users to quickly master the remote control programming method of the 87235.

- Error Description

Error message description and method to obtain after-sales services are included.

- Appendixes

Necessary reference information related to program control of the 87235 is provided, including zoom table of SCPIs.

1.2 Related Documents

The product documentation includes

- Quick Start Guide
- User's Manual
- Program Control Manual

Quick Start Guide

This manual introduces the basic methods for configuration and start-up measurement of the instrument to enable users to quickly understand the characteristics of the instrument, and master the basic settings and basic operation methods. Main chapters include:

- Get Prepared
- Typical Applications
- Get Help

User's Manual

This manual describes the functions and operation methods of the analyzer in detail, including configuration, measurement, program control and maintenance, etc. The purpose is to guide users to fully understand the functional characteristics of the product and master common testing methods of the instrument. Main chapters include:

- Manual Navigation
- Overview
- Quick Start
- Operation Guide
- Menus
- Remote Control
- Troubleshooting and Repair
- Technical Indicators and Testing Methods
- Appendixes

Program Control Manual

This manual introduces remote programming basics, SCPI basics, SCPI, programming examples and I/O driver function library in detail. The purpose is to guide users to quickly and comprehensively master the program control commands and methods of the instrument. Main chapters include:

- Remote Control
- Program Control Commands
- Programming Examples
- Error Description
- Appendixes

2 Remote Control

This chapter introduces the remote control basics, remote control interface and configuration methods of the 87235, and briefly introduces the concept and classification of I/O instrument driver library. The purpose is to facilitate users to start to achieve remote control. Specific contents include:

- Remote Control Basics....3
- Instrument Program Control Port and Configuration....29
- I/O Library....31
- Zeroing....31
- Performing Measurements....32
- Using Frequency Response Offset Table....32
- Setting Display Resolution....34
- Setting Average....35
- Setting Offset....35
- Setting Measurement Limit....35
- Status Report....36
- Storage/Loading....37

2.1 Remote Control Basics

- Program Control Interface....3
- Message....7
- SCPI Command....8
- Command Sequence and Synchronization....19
- Status Reporting System....21
- Programming Considerations....29

2.1.1 Program Control Interface

- LAN Interface....4
- GPIB Interface....6
- RS-232 Interface....6
- USB Interface....7

Instruments with remote control function generally support two kinds of remote control interface: LAN, GPIB, RS-232 and USB, and the type of port supported by the specific model of instrument is determined by the function of the instrument.

The remote control interface and related VISA addressing string are described in the table below:

Table 2.1 Remote control interface type and VISA addressing string

Program control interface	VISA addressing string	Description
LAN (Local Area Network)	VXI-11 protocol: TCPIP::Addressograph[::LAN_device_name][::INSTR] Raw socket protocol: TCPIP::Addressograph::port::SOCKET	The controller realizes remote control by connecting the instrument with the network port on the rear panel of the instrument. For details of the protocol, please refer to: 2.1.1.1 LAN interface
GPIB (IEC/IEEE Bus Interface)	GPIB::primary address[::INSTR]	The controller realizes remote control by connecting the instrument with the port on the rear panel of the instrument. Follow the bus interface standard IEC 625.1/IEEE 418. For details, please refer to: 2.1.1.2 GPIB interface
RS-232 (Recommended Standard-232)		Instrument rear panel port. For details, please refer to: 2.1.1.3 RS-232 Interface
USB (Universal Serial Bus)	USB::<vendor ID>::<product_ID>::<serial_number>[::INSTR]	Instrument rear panel port. For details, please refer to: 2.1.1.4 USB interface

2.1.1.1 LAN interface

An instrument with a network interface (hereinafter referred to as instrument) can be controlled remotely by computers in 10Base-T and 100Base-T. Various instruments are combined into a system in LAN and controlled uniformly by computers in it. In order to realize remote control in LAN, it should be equipped with port connector, network card and relevant network protocol in advance, and provided with relevant network services. Meanwhile, the host computer in the network should also be equipped with instrument control software and VISA library in advance. The three working modes of the network card are:

- 10Mbit/s Ethernet IEEE802.3;
- 100Mbit/s Ethernet IEEE802.3u;
- 1Gbit/s Ethernet IEEE802.3ab.

The host computer and the instrument should be connected to the common TCP/IP protocol network through the network port. The cable between the computer and the instrument is a commercial RJ45 cable (Category 5 cable with or without shielding). During data transmission, the transmission speed of LAN is faster when data packet transmission is applied. Generally, the length of the cable between the computer and the instrument should not exceed 100m (100Base-T and 10Base-T). For more information about LAN communications, please refer tohttp://www.ieee.org.

Knowledges about the LAN interface are introduced below:

1) IP address

Physical connection of the network should be guaranteed for remote control on the instrument via the LAN. It is just required to set the address to the subnet in which the host computer is located via the network configuration interface of the instrument. For example, if the IP address of the host computer is 192.168.12.0, the IP of the instrument shall be set to 192.168.12.XXX, whereas XXX is the figure between 1 and 255.

When establishing a network connection, only the IP address is required. The VISA addressing string is as follows:

TC PIP::host address[::LAN device name][::INSTR] or

TCPIP: : host address: port: : SOCKET

Where:

- TCPIP represents the network protocol used;
- host address represents the IP address or host name of the instrument, and is used for identifying and controlling the controlled instrument;
- LAN device name defines the handle number of the protocol and subset (optional);
  - VXI-11 protocol is selected for device 0;
  - More recent high speed LAN instrument protocol is selected for high speed LAN instrument 0;
- INSTR represents the instrument resource type (optional);
- port represents the socket port number;
- SOCKET represents the raw network socket resource class.

Example:

- The IP address of the instrument is 192.1.2.3, and the effective resource string of the VXI-11 protocol is:

  TCPIP::192.1.2.3::INSTR

- To establish a raw socket connection, use:

  TCPIP::192.1.2.3::5025::SOCKET

TIPS

Method of recognizing multiple instruments in the program control system

If multiple instruments are connected in the network, the individual IP address and related resource string are used to distinguish. The host computer applies its own VISA resource string for instrument identification.

2) VXI-11 protocol

The VXI-11 standard is based on the ONC RPC (Open Network Computing Remote Procedure Call) protocol, which is the network/transport layer of the TCP/IP protocol. The TCP/IP network protocol and associated network services are pre-configured for communication. Such connection-oriented communication, which follows the sequential exchange and can identify the interruption of the connection, ensures no loss of

information.

3) Socket communication

The TCP/IP protocol connects the instrument to the network via LAN sockets. As a basic method used in computer network programming, the socket allows applications using different hardware and operating systems to communicate over a network. With this method, two-way communication between the instrument and the computer is realized through ports.

As a software class programmed specially, the socket defines the IP address, device port number and other necessary information for network communication, and integrates some basic operations in network programming. Sockets can be used after installing packaged libraries in the operating system. Two commonly used socket libraries are the Berkeley socket library for UNIX the Winsock library for Windows.

Sockets in the instrument are compatible with Berkeley sockets and Winsock through the application program interface (API). In addition, it is compatible with the API of other standard sockets. When SCPI are used to control the instrument, the socket program established in the program issues the command. Before using a LAN socket, the socket port number of the instrument must be set. The socket port number of the instrument is 5025.

2.1.1.2 GPIB interface

As an instrument remote control interface widely used at present, GPIB interface is connected to different types of instruments through GPIB cable, so as to build a test system with the host computer. In order to realize remote control, the host computer should be equipped with GPIB bus card, driver and VISA library in advance. During communication, the host computer first addresses the controlled instrument through the GPIB bus address. The user may set the GPIB address and ID query string, and the GPIB communication language may be in the form of SCPI by default.

GPIB and its associated interface operations are defined and described in detail in ANSI/IEEE Standard 488.1--2003 and ANSI/IEEE Standard 488.2--1992. For details of the standards, please refer to the IEEE website: http://www.ieee.org.http://www.ieee.org

GPIB processes information in bytes at the data transmission speed of up to 8MBps, which is fast. Since the data transmission rate is limited by the distance between the device/system and the computer, the following points should be noted when connecting GPIB:

- Up to 15 instruments may be built through GPIB interface.
- The total length of the transmission cable should not be more than 15 m or twice the number of instruments in the system. In general, the maximum length of the transmission cable between the devices shall not exceed 2 m;
- If multiple instruments are connected in parallel, a "live" cable is required;
- The end of the IEC bus cable shall be connected to the instrument or host computer.

2.1.1.3 RS-232 interface

RS-232 is a traditional method to realize program control. Because it only sends and receives one bit of data at a time, the transmission rate is slower than GPIB or LAN, which is not commonly used at present. Similar to GPIB and LAN, instrument parameters, such as baud rate, need to be set when establishing communication in order to match the parameters with the host computer. RS-232 transmits SCPI command characters in ASCII form.

2.1.1.4 USB interface

To implement USB programming, a computer and signal generator need to be connected via a USB port with the VISA library installed in advance. VISA automatically detects and configures the instrument to establish a USB connection without the need to enter the instrument address string or install a separate driver.

USB Address:

Addressing string format: USB::<vendor ID>::<product ID>::<serial number>[::INSTR]

Where:

- <vendor ID> represents the manufacturer code;
- <product ID> represents the instrument code;
- <serial number> represents the serial number of the instrument;

Example:

USB::1204::4112::SN100001::INSTR

1204: Manufacturer designator, which can be expressed as 0x4b4 in hexadecimal;

4112: Instrument designator, which can be expressed as 0x1010 in hexadecimal;

SN100001: Serial number of the instrument.

2.1.2 Message

The messages transmitted on the data cable are divided into the following two categories:

1) Interface message

During communication between the instrument and the host computer, the attention cable should be pulled down first, and then the interface message will be transmitted to the instrument through the data cable. Only instruments with GPIB bus function can send interface message.

2) Instrument message

For the detailed structure and syntax of the instrument message, see Section "2.1.3 SCPI command". The instrument message can be divided into two types as per the transmission direction, namely, command and instrument response. Unless otherwise stated, all remote control interfaces apply instrument message in the same way.

a) Commands:

Commands (programming messages) are messages sent by the host computer to the instrument for remote control of instrument functions and query of status information. Commands are divided into the following two categories:

- Based on the impact on the instrument:
  - setting commands: change the set state of the instrument, such as reset or setting frequency.
  - query commands: query and return data, for example: identify the instrument or query the parameter value. Query commands end with the suffix question mark.
- Based on the definition in the standard:

- common commands: with functions and syntax to be defined by IEEE488.2, they are applicable to all types of instruments (if realized)
- The purpose is for management of standard status register, reset and self-detection, etc.
- instrument control commands: instrument characteristic commands, used to realize instrument functions, such as setting frequency.

  The syntax also follows the specifications of SCPI.

b) Instrument responses:

Instrument responses (response message and service request) are the query result information sent by the instrument to the computer. Such information includes measurement results, instrument status, etc.

2.1.3 SCPI

- Introduction to SCPI.....8
- Description of SCPI.....9

2.1.3.1 Introduction to SCPI Command

SCPI (Standard Commands for Programmable Instruments) are a command set for all instruments established based on Standard IEEE488.2. The main purpose is to make the same function have the same program command to achieve the universality of program control commands.

SCPI consist of a command header and one or more parameters. The command header is separated from the parameters by spaces and contains one or more key fields. A command with direct suffix question mark is a query command. Commands are divided into common commands and instrument commands that have different syntactic structures. SCPI have the following characteristics:

1) Program control commands are oriented to test function rather than describing instrument operation;

2) Program control commands reduce the repetition of similar test function realization process, and ensure the compatibility of programming.

3) Program control messages are defined in layers that are hardware independent of the communication physical layer;

4) Program control commands are independent of programming methods and languages. The test program of SCPIs is easy to transplant;

5) Program control commands are scalable and can adapt to different scale of measurement control;

6) SCPI have been a “living” standard for their scalability.

If you are interested in learning more about SCPI, please refer to:

IEEE Standard 488.1-2003, IEEE Standard Digital Interface for Programmable Instrumentation. New York, NY, 1998.

IEEE Standard 488.2-1992, IEEE Standard Codes, Formats, Protocols and Comment Commands for Use with ANSI/IEEE Std488.1-2003. New York, NY, 1998

Standard Commands for Programmable Instruments(SCPI) VERSION 1999.0.

For program control command set, classification and description of the 87235, please refer to:

1) "3. Program control commands" in this Manual;

2) “Appendix A Zoom Table of SCPI commands classified as per subsystems” of the Manual.

2.1.3.2 Description of SCPI

- General Terms.....9
- Command Type.....10
- Instrument Command Syntax.....10
- Command Tree.....14
- Command Parameters and Responses.....14
- Number System of Commands.....18
- Command Line Structure.....18

1) General terms

The following terms apply to this section. To better understand the chapters, you shall understand the exact definitions of the terms.

Controller

A controller is any computer used to communicate with the SCPI device. A controller may be a PC, minicomputer, or a plug-in card on a cage. Some AI devices can also be used as controllers.

Device

A device is any device that supports SCPI. Most of the devices are electronic measurement or excitation devices that use GPIB interfaces for communication.

Program message

A program message is the combination of one or more SCPI commands that have been correctly formatted. Program messages tell the devices how to measure and output the signals.

Response message

A response message is a set of data of specified SCPI formats. Response messages always come from the devices to controllers or listening devices. Response messages tell the controllers about the internal state or measured values of the devices.

Command

A command is an instruction that satisfies the SCPI standard. The combination of commands controlling the devices forms a message. In general, a command includes keywords, parameters, and punctuation.

Event command

Event-type program control commands cannot be queried. An event command generally has no corresponding front panel key setting, and its function is to trigger an event at a specific time.

Query

A query is a special type of command. When a control device is queried, a response message appropriate to the controller syntax requirements is returned. A query statement always ends with a question mark.

2) Command type

There are two types of SCPI: common commands and instrument commands. Figure 2.1 shows the difference between the two commands. Common commands, defined by IEEE 488.2, are used to manage macros and status registers and for synchronization and data storage. Because common commands all start with an asterisk, they are easy to be recognized. For example, *IDN?, *OPC, *RST are all common commands. Common commands are not part of any instrument commands, and the instrument interprets them in the same way regardless of the current path setting of the commands.

Instrument commands are easy to be recognized because they contain a colon (:). A colon is used in the beginning of an expression or between two keywords, for example: FREQuency[:CW?]. According to the internal function module of the instrument, instrument commands are divided into sub-sets of corresponding subsystem commands. For example, the power subsystem (:POWer) contains power-related commands, while the status subsystem (:STATus) contains commands for the status control register.

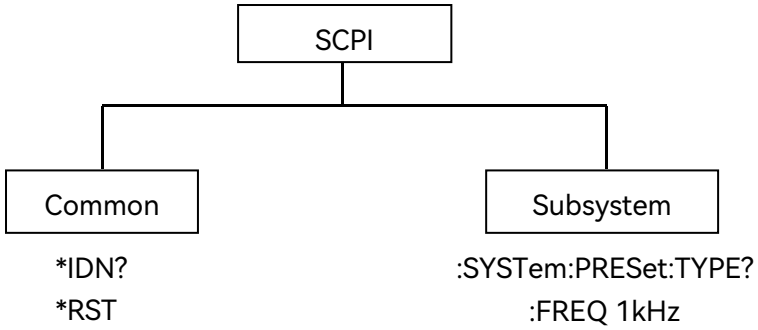


Figure 2.1 Types of SCPI

3) Instrument Command Syntax

A typical command consists of a keyword prefixed with a colon. The keyword is followed by parameters. The following is an example of a syntax declaration:

[:SENSe:]FREQuency[:CW|FIXed] MAXimum|MINimum

In the example above, the [:CW|FIXed] in the command follow : FREQuency closely without any space. MINimum|MAXimum immediately following [:LEVel] is the parameter. There is a space between the command and the parameter. Other parts of the syntax expression are described in Table 2.2 and Table 2.3.

Table 2.2 Special characters in command syntax

Symbol	Meaning	Example
|	The vertical bar between the keyword and the parameter represents multiple options.	[:SENSe:]BANDwidth|BWIDth HIGH|LOWer BANDwidth and BWIDth are optional; HIGH and LOWer are optional.
[]	A square bracket indicates that the contained keyword or parameter is optional when forming a command. The command will be executed even when such implied keyword or parameter is ignored.	[:SENSe:]BANDwidth? SENSe is optional.
< >	The part in angle brackets indicates that the command is not used in the literal sense. They represent the part that must be contained.	[:SENSe:]FREQency[:CW|FIXed] <val>[unit] In this command, <val> must be replaced with actual frequency. [unit] is an omittable unit. For example: FREQ 3.5GHz FREQ 3.5e+009
{ }	The part in braces indicates that the parameter is optional.	MEMory:TABLe:FREQuency <val>{,<val>} For example: MEM:TABL:FREQ 5e7

Table 2.3 Command syntax

Characters, keywords and syntax	Example
Uppercase characters represent the minimum set of characters required to execute a command.	[:SENSe:]FREQuency[:CW|FIXed]?, FREQ is the short format part of the command.
Lowercase character of the command is optional; such flexible format is called "flexible listening". See the section "Parameters and Responses of Commands" for more information.	:FREQuency :FREQ,:FREQuency or or :FREQUENCY Either of them is correct.
When a colon is between the two command mnemonics, it moves the current path in the command tree down by one level. For more information, please refer to the command path part in section “Command Tree”.	:TRIGger:MODE? TRIGger is the topmost keyword of this command.
If the command contains more than one parameter, adjacent parameters are separated. The parameter is not part of the command path, so it does not affect the path layer.	MEMory:TABLe:FREQuency <val>{,<val>}
The semicolon is used to separate 2 adjacent	:FREQ 2.5GHZ; :POW 10DBM

commands, without affecting current command path.	
Blank characters, such as <space> or <tab>, are usually ignored as long as they do not appear between keywords or in keywords. However, you must separate the commands and parameters with blank characters, which does not affect the current path.	:FREQuency or :POWer :LEVel6.2 is not allowed. :LEVel and 6.2 must be separated by a space, namely, :POWer:LEVel 6.2.

The simplified syntax specification is shown in Figure 2.2.

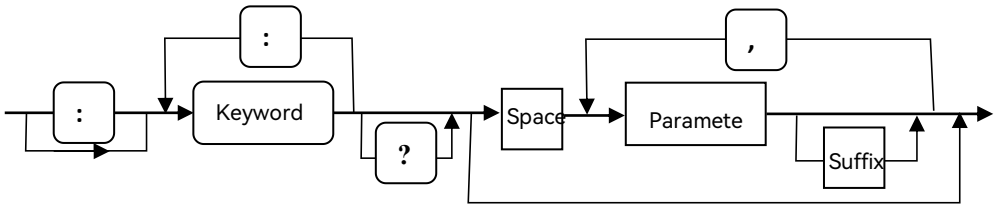


Figure 2.2 Types of SCPI

For example, the syntax expression of "[:SENSe[1]:]FREQuency[:CW|FIXed] <numeric parameter>" can be expressed as follows.

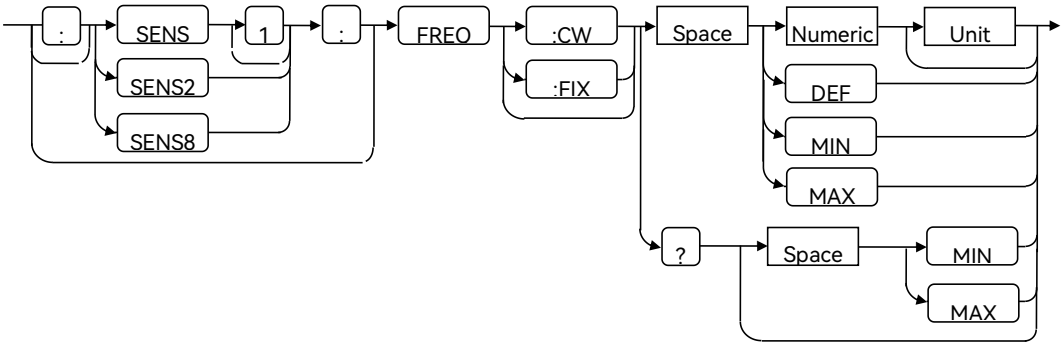


Figure 2.3 Types of SCPI

Remarks:

1) In the above chart, no spaces may be added where spaces are not indicated as required. Spaces may be 1 or more. If the units are omitted, the standard unit of frequency, Hz, and the standard unit of time, seconds, are used.

2) Rounded rectangles indicates the actual characters required for the keywords or commands, such as ":", ",", "?" , "1", etc.; Right-angled rectangles need to be replaced by actual characters, numbers, etc. For example, the "value" cannot appear in the command, and it needs to be replaced by the actual value, such as 5e+007, etc.

3) Without considering the short and long format of the keyword, the frequency of Channel A is set to 50MHz, and the above chart has the following forms (only the short format of the keyword is taken. Since there are many units of frequency, such as Hz, kHz, MHz, GHz, THz, etc., it is no longer given one by one due to space limitations. It is only necessary to replace 5.0e+007 with corresponding units, such as 50MHz, 5e+007Hz, 0.05GHz, etc.).

   a) :SENS1:FREQ:CW 5.0e+007 No keywords omitted

b) SENS1:FREQ:CW 5.0e+007 The ":" before SENS1 omitted.

c) SENS:FREQ:CW 5.0e+007 "1" omitted.

d) FREQ:CW 5.0e+007 SENS omitted.

e) :SENS1:FREQ:FIX 5.0e+007 No keywords omitted

f) SENS1:FREQ:FIX 5.0e+007 The ":" before SENS1 omitted.

g) SENS:FREQ:FIX 5.0e+007 "1" omitted.

h) FREQ:FIX 5.0e+007 SENS omitted.

i) :SENS1:FREQ 5.0e+007 CW or FIX omitted

j) SENS1:FREQ 5.0e+007 The ":" before SENS1 and CW or FIX

k) SENS:FREQ 5.0e+007 "1" and CW or FIX omitted.omitted.

l) FREQ 5.0e+007 SENS and CW or FIX omitted.

4) For Channel B and channel 8 frequencies, SENS2 and SENS8 cannot be omitted.

5) MIN and MAX can be used as parameters of the set command or as parameters of the query command. DEF can only be used as a parameter of the set command. The specific values of MIN, MAX, and DEF are related to the instrument.

a) FREQ DEF Set the frequency of Channel A to the default value.

b) FREQ? MAX Query the maximum settable frequency of Channel A and return a value without unit.

6) If the long and short forms of keywords are considered, and commands with units are not considered, there are 1632 forms of commands in the above chart. Users don't have to care about all forms. As long as it can be used flexibly, it is enough. A simple calculation is performed below, and interested users can calculate by themselves.

a) First calculate the case where SENS is defaulted, noted as N1.
There are 2 forms of FREQ/FREQuency, noted as N11.
There are four forms of CW/FIX/FIXed/Omitted, noted as N12.
There are 7 parameters of the set command:
Value/DEF/DEFault/MIN/MINimum/MAX/MAXimum.
The parameters of the query command are
MIN/MINimum/MAX/MAXimum/Omitted, i.e., there are 12 types of parameters, which are recorded as N13, then
$$N1 = N11 \times N12 \times N13 = 2 \times 4 \times 12 = 96$$

b) Then calculate the case where SENS is not defaulted, noted as N2.
The first ":" has 2 types, omitted and not omitted, noted as N21.
There are 2 types of SENS/SENSe. There are 4 types of suffixes: 1/2/6/Omitted, i.e., there are 8 (2×4) types of SENS keywords, noted as N22.
SENS keyword forms a combination with the following keywords, then
$$N2 = N21 \times N22 = 2 \times 8 \times N1 = 16 \times N1$$

c) Let there be a total of N forms, then
$$N = N1 + N2 = 17 \times N1 = 1632$$

4) Command tree

Most remote control programs apply instrument commands. When parsing such commands, SCPI apply a file system-like structure called command tree, as shown in Figure 2.4:

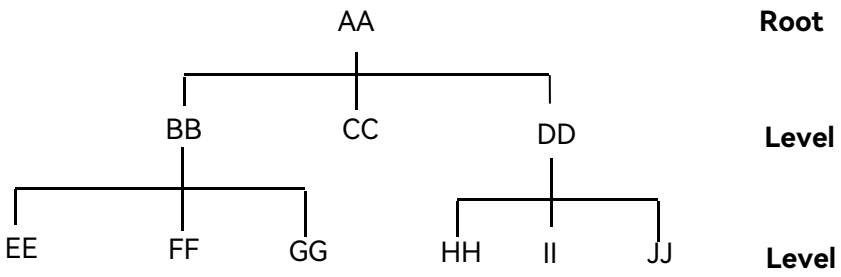


Figure 2.4 Diagram of the simplified command tree

The top command is the root command, or "root" for short. When a command is parsed, follow a specific path to the next level of command according to the tree structure. For example, in :POWer:ALC:SOURce?, : POWer stands for AA, :ALC stands for BB, :SOURce stands for GG, and the entire command path is (:AA:BB:GG).

A software module in instrument software – **command interpreter**, is responsible for parsing each received SCPI. The command interpreter breaks commands into individual command elements by using a series of rules that distinguish the path of the command tree. After parsing the current command, keep the current command path unchanged. The advantage of this is to parse subsequent commands more quickly and efficiently since that the same command keyword may appear in different paths. After booting or *RST (reseting) the instrument, current command path is reset to root.

5) Command parameters and responses

SCPI define different data formats in the use of program and response messages to comply with the principles of "***flexible listening***" and "***precise speaking***". For more information, please refer to IEEE488.2. "***Flexible listening***" means that the formats of the commands and parameters are flexible.

For example, to set the frequency offset status command :FREQuency:OFFSet:STATe ON|OFF|1|0.

The following command formats are all used to set the frequency offset function to on:

:FREQuency:OFFSet:STATe ON, :FREQuency:OFFSet:STATe 1,

:FREQ:OFFS:STAT ON, :FREQ:OFFS:STAT 1

Each parameter type has one or more corresponding response data types. During query, a data type will be returned for a numerical parameter, and the response data is precise and strict, known as "**precise speaking**."

For example, during query of the power state (:POWer:ALC:STATe?), when it is ON, the response data returned is always 1 during query, regardless of whether the previously sent setting command is :POWer:ALC:STATe 1 or :POWer:ALC:STATe ON.

Table 2.4 Parameter and response types of SCPI

Parameter type	Response data type
Numerical	Real number or integer
Extended numerical	Integer
Discrete	Discrete
Boolean	Digital boolean
String	String
Blocks	Finite-length blocks
	Infinite-length blocks
Non-decimal numeric types	Hexadecimal
	Octal
	Binary

Numerical parameters

Numeric parameters can be used in both instrument-specific commands and common commands. A numeric parameter receives all the usual decimal counting methods, including signs, decimals, and scientific notation. If a device only accepts a specified numeric type, such as an integer, it will automatically round up the received numeric parameters.

Examples of numeric parameters:

0	No decimal point
100	Optional decimal point
1.23	Signed bit
4.56e<space>3	Index mark e can be followed by a space
-7.89E-01	Index marker e can be uppercase or lowercase
+256	Positive lookahead allowed
.5	Decimal points can be used first

Extended numerical parameters

Most measurements related to instrument commands use extended numeric parameters to specify physical quantities. Extended numerical parameters receive all numeric parameters and additional special values. All the extended numeric parameters receive MAXimum and MINimum as parameter values. Whether other special values, such as UP and DOWN, will be received is determined by the ability of the instrument to parse. All effective parameters will be listed in the table of SCPI.

Note: Extended numeric arguments do not apply to common commands or STATus subsystem commands.

Examples of extended numeric parameters:

101	Numeric parameter
1.2GHz	GHz can be used as an index (E009)

200MHz	MHz can be used as an index (E006)
-100mV	-100 millivolts
10DEG	10 degrees
MAXimum	Maximum effective setting
MINimum	Minimum effective setting
UP	Increase by a step
DOWN	Reduce by a step

Discrete parameters

When the number of parameter values to be set are finite, they are identified by discrete parameters. Discrete parameters use mnemonics to represent each valid setting. Like program command mnemonics, discrete parameter mnemonics have two formats, long and short, and allow for mixture of upper and lower cases.

In the following examples, discrete parameters and commands are used together.

:TRIGger[:SEQuence]:SOURce BUS|IMMediate|EXTernal

BUS GPIB, LAN, RS-232 trigger

IMMediate Trigger immediately

EXTernal Trigger externally

Boolean parameters

A Boolean parameter represents a true or false binary condition, which can only have four possible values.

Examples of Boolean parameters

ON	Logically true
OFF	Logically false
1	Logically true
0	Logically false

String parameters

String parameters allow ASCII strings to be sent as parameters. Single quotes and double quotes are used as separators.

The following are example of string parameters:

'This is Valid' "This is also Valid" 'SO IS THIS'

Real response data

Most of the test data are of real number type, and their formats can be basic decimal notation or scientific notation, which are supported by most advanced programming languages.

Examples of real response data:

1.23E+0

-1.0E+2

+1.0E+2

0.5E+0

0.23

-100.0

+100.0

0.5

Integer response data

An integer response data is a decimal expression of an integer value containing signed bit. When querying the status register, most of the response data returned are of integer type.

Examples of integer response data:

0	Sign bit optional
+100	Positive lookahead allowed
-100	Negative lookahead allowed
256	No decimal point

Discrete response data

Discrete response data are basically the same as discrete parameters, only that the return format of discrete response data is only a short form in uppercase.

Examples of discrete response data:

INTernal	Stabilization mode is internal
EXTernal	Stabilization mode is external
MMHead	Stabilization type is millimeter wave source module

Digital Boolean response data

A binary value 1 or 0 is returned as Boolean response data.

String response data

String response data and string parameters are alike. The main difference is that the separators of string response data are double quotes instead of single quotes. Double quotes can also be embedded in string response data, and there may be no characters between the double quotes.


Here are some examples of string response data:

“This is a string”

“one double quote inside brackets: (“”)”

Arbitrary data block

See Section 7.7.6 of IEEE 488.2 for <Arbitrary data block>.

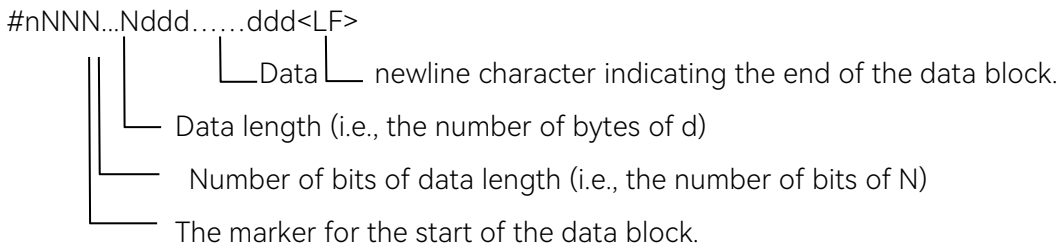

For example: #42004 ..... in <LF> n = 4 and N = 2004.

6) Number system of commands

The value of the command can be entered in binary, decimal, hexadecimal or octal format. When using binary, hexadecimal or octal format, a proper identifier is required before the value. The decimal format (the default format) does not require an identifier. When a value is entered without an identifier in front of it, the device will ensure it to be in decimal format. The following list shows the identifiers required for different formats:

#B indicates that the number is a binary number;

#H indicates that the number is a hexadecimal number;

#Q indicates that the number is an octal number.

The following are various representations of the decimal number 45 in SCPI:

#B101101

#H2D

#Q55

The following example sets the RF output power to 10 dBm (or a value of the equivalent value of the currently selected unit, such as DBUV or DBUVEMF) with a hexadecimal value of 000A.

:POW #H000A

When using a non-decimal format, a measurement unit, such as DBM or mV, is not used with the value.

7) Command line structure

A command line may contain multiple SCPI. To indicate the end of the current command line, the following methods may be used:

- Line feed;
- Line feed and EOI;
- EOI and the last data byte.

Commands on the command line are separated by semicolons, and commands belonging to different subsystems begin with a colon. For example:

MMEM:COPY "Test1", "MeasurementXY";:HCOP:ITEM ALL

The command line contains two commands: the first one belongs to the MMEM subsystem, and the second belongs to the HCOP subsystem. If adjacent commands belong to the same subsystem with repeated command path, they can be expressed in abbreviation. For example:

HCOP:ITEM ALL;:HCOP:IMM

The command line contains two commands: both of them belong to the HCOP subsystem, with the same first level. Therefore, the second command can start from the next level of HCOP, and the colon for starting the command can be omitted. It can be abbreviated as follows:

HCOP:ITEM ALL;IMM

2.1.4 Command Sequence and Synchronization

IEEE488.2 defines the difference between overlapping and sequential commands:

- Sequential commands are sequences of commands that are executed continuously. Each command is usually executed faster;
- An overlapping command is one that is not executed automatically before the next command is executed. It usually takes longer to process overlapping commands, and programs are allowed to process other events synchronously during the period.

Even if there are multiple setting commands on a command line, they may not be executed in the order they were received. To ensure that commands are executed in a certain order, each command must be sent on a separate command line.

Example: the command line contains setting and query commands

If multiple commands on a command line contain query commands, the query results are unpredictable. A fixed value is returned for the following command:

:FREQ:STAR 1GHZ;SPAN 100;:FREQ:STAR?

Returned value: 1000000000 (1GHz)

The following command returns an unfixed value:

:FREQ:STAR 1GHz;STAR?;SPAN 1000000

The returned result may be the current starting frequency value because the host program will delay execution of the command. If the host program executes after receiving the command, the returned result may also be 1GHz.

TIPS

Setting commands are sent separately from query commands

General rules: in order to ensure the correctness of returned results of query commands, setting commands and query commands should be sent in different program messages.

2.1.4.1 Prevent Overlapping Execution of Commands

In order to prevent overlapping execution of commands, multithreading or commands *OPC, *OPC? or *WAI may be applied, which are executed only after the hardware setting is completed. During programming, the computer may force a period of time to synchronize certain events. The descriptions are shown below:

- The controller program applies multi-threading

Multi-threading is used to wait for command completion and synchronization between the UI and program control, that is, to wait for *OPC? Completion in separate threading without interfering GUI or program threading execution.

➢ The application of the three commands in synchronous execution is shown in the table below:

Table 2.5 Command usage

Method	Action	Programming method
*OPC	After the command is executed, set it in the operation completion bit of the ESR register.	Set to ESE BIT0; Set to SRE BIT5; Send overlapping commands and *OPC; Wait for service request (SRQ); Service request represents that the overlapping command has been executed.
*OPC?	Stop executing the current command until 1 is returned. The command is returned only when it is in the operation completion bit of the ESR register, indicating that the previous command has been processed.	Terminate processing of the current command before executing other commands, and send the command directly after the current command.
*WAI	Before the execution of *WAI, wait for all commands to be sent before proceeding with unfinished commands.	Terminate the processing of the current command before executing other commands, and send the command directly after the current command.

In the case that the processing time of overlapping command is short, the command *WAI or *OPC may be used after the overlapping command to achieve command synchronization. In order to execute other tasks synchronously while the computer or instrument is waiting for the completion of overlapping commands, the following synchronization techniques may be applied:

➢ OPC and service request

1) Set the OPC mask bit of ESE (bit0): *ESE 1;

2) Set the bit5 of SRE: *SRE 32 enable ESB service request;

3) Send overlapping commands and *OPC;

4) Wait for service request.

Service request represents that the overlapping command has been executed.

➢ OPC? and service request

1) Set the bit4 of SRE: *SRE 16 enable MAV service request;

2) Send overlapping commands and *OPC?;

3) Wait for service request.

Service request represents that the overlapping command has been executed.

➢ Event status register (ESE)

1) Set the OPC mask bit of ESE (bit0): *ESE 1;

2) Send only overlapping commands instead of *OPC, *OPC or *WAI;

3) Send "*OPC;*ESR?" in timer for cyclic query of the operation status.

The returned value (LSB) 1 indicates completion of the overlapping command.

➢ * OPC? and short timeout

1) Send only overlapping commands instead of *OPC, *OPC or *WAI;

2) Send "<short timeout>; *OPC?" in timer for cyclic query of the operation status;

3) A return value (LSB) equal to 1 indicates that the execution of the interleave command is complete. In case of timeout, it is during operation.

4) Reset the timeout value to the old value;

5) Send the command "SYStem:ERRor?" to clear the error queue, and delete the message "-410, query interrupt".

The returned value (LSB) 1 indicates completion of the overlapping command.

2.1.5 Status Reporting System

The status reporting system stores all operation status information for the current instrument, including error message. They are stored in status registers and error queues respectively, and can be queried through a remote control interface.

- Structure of Status Register.....21
- Structure of SCPI Status Register.....22
- Description of Status Register.....23
- Application of Status Reporting System.....26
- Reset Status Reporting System.....28

2.1.5.1 Structure of Status Register

Status registers are described by classification below:

1) STB, SRE

The status byte (STB) register and its related mask register - service request enable register (SRE), comprise the top register of the status reporting system. STB saves the general working state of the instrument by collecting the information of lower registers.

2) ESR, SCPI status register

➢ STB receives information from the following registers:

➢ The value of the event status register (ESR) and the event status enable (ESE) mask register.

SCPI status register includes: STATus:OPERation and STATus:QUEStionable registers (SCPI definition),

which contain the specific operation information of the instrument. All SCPI status registers have the same internal structure(For details, see 2.1.5.2 "SCPI status register structure"of the program control manual).

3) IST,PPE

Similar with SRQ, IST ("Individual Status") marks a separate bit consisting of all statuses of the instrument. The associated parallel poll enable register (PPE) determines the STB

data bits for IST marking.

4) Output buffer

It stores the messages returned by the instrument to the master. It does not belong to the status report system, but determines the MAV position value of the STB.

TIPS

SRE, ESE

SRE may be used as the enable part of STB. Similarly, ESE may be used as the enable part of ESR.

2.1.5.2 Structure of SCPI Status Register

Each standard SCPI register consists of five parts. Each part contains 16 bits and is functionally independent. For example, one bit is assigned for each hardware status and valid for all five parts of the register. If Bit15 is set to 0, the value of the register is positive integer data.

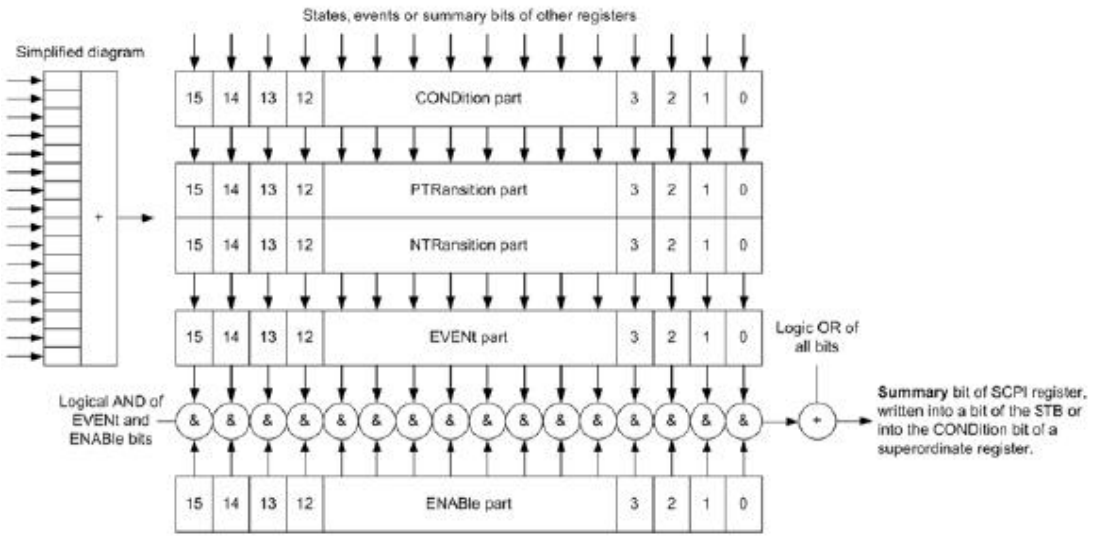


Figure 2.5 Structure of status register

It can be seen from the figure above that the status register consists of five parts, which are respectively described as follows:

- Condition register

In this part, the summary bit of hardware or lower registers are directly written, reflecting the working state of the current instrument. This register is read only, not writable. It reads but not clearing the value.

- Positive/negative transition register

The two transition registers define the state transition bit of the condition register stored in the event register.

The positive transition register is similar to the transition filter. When a bit of the

condition register is transformed from 0 to 1, relevant PTR bit determines whether the event bit is set to 1, as shown below:

— PTR bit = 1: the event bit is set.

— PTR bit =0: the event bit is not set.

The positive transition register is readable and writable. It reads but not clearing the value.

The negative transition register is similar to the transition filter. When a bit of the condition register is transformed from 1 to 0, relevant NTR bit determines whether the event bit is set to 1, as shown below:

— NTR bit = 1: the event bit is set.

— NTR bit = 0: the event bit is not set.

The positive transition register is readable and writable. It reads but not clearing the value.

➢ Event register

This part indicates whether the event has occurred since the last reading and whether the content of the condition register is stored. It represents only the event passed through the transition register. It can only be changed by the instrument and read by the user. The value will be cleared after reading. The value of this part is often equal to the value of the entire register.

➢ Enable register

This part determines whether the related event bit acts on the final summary data. The bits of each enable part is the sum of related enable bits. The logical operation result of this part is or not the summary bit.

— enable bit = 0: the related event bit does not act on the summary data.

— enable bit = 1: the related event bit acts on the summary data.

This part is readable and writable. It reads but not clearing the value.

➢ Summary bit

The summary bit of each register consists of the event and the enable part. The result enters the condition part of the upper register. The instrument automatically generates the summary bit for each register so that events can cause different levels of service requests.

2.1.5.3 Description of Status Register

The status registers are detailed as follows:

1) Status byte (STB) and service request enable register (SRE)

IEEE488.2 defines the status byte (STB). The rough instrument status is reflected by collecting the information of lower registers. Bit6 is equal to the summary data of other status byte bits. The result of a comparison between the status byte and the condition part of the SCPI register may be assumed to be the top in the SCPI hierarchy. The value of status byte may be read through common command "*STB?" or serial query.

The status byte is connected to the service request enable register (SRE). Each bit of the status byte corresponds to a bit in SRE. Bit6 of SRE is ignored. If one of the bits in SRE is set and the related STB bit changes from 0 to 1, a service request (SRQ) will be

generated. Common command "*SRE" is used to set SRE, and common command "*SRE?" used to read SRE. The status byte is described in Table 2.6 Description of status byte:

Table 2.6 Description of status byte

Bit	Meaning
0	Not used.
1	Device related.
2	The error queue is not empty Set to this bit when a new error is inserted into the error queue. If related SRE bit enables the bit, a service request will be generated when a new error is generated in the error queue, so that the error can be identified and the error message can be queried. Such method effectively reduces errors in program control.
3	Summary bit of inquiry status register Set to this bit only when the event bit of the inquiry status register and the related enable bit are set to 1. This bit represents a queriable status of the instrument. Specific instrument status information can be obtained by querying the inquiry status register of the status register.
4	MAV bit (message available) Set to this bit if the output queue information is readable. This bit is used when the controller queries instrument information.
5	ESB bit Summary bit of the event status register. Set to this bit when one of the bits in the event status register is set and the corresponding bit in the event status enable register is enabled. The bit of 1 indicates a serious error in the instrument. The specific error message can be found by querying the event status register.
6	MSS bit (master status summary bit) Set this bit if the instrument triggers a service request.
7	Summary bit of operation status register Set to this bit when the event bit of the operation status register and the corresponding enable bit are set to 1. This bit indicates that the instrument has performed an operation, the type of which can be obtained by querying the operation status register.

2) IST flag and parallel poll enable (PPE) register

The IST identifies the combination of the overall instrument state with a single data bit. The flag can be obtained by a parallel poll or by sending the command "*IST?". The associated parallel poll enable register (PPE) determines the STB data bits for IST marking. STB data bits are in phase with PPE data bits, and the usage of bit6 is opposite to bit6 in SRE. The IST flag is equal to the threshold of all results. The command "*PRE" may be used to set PPE, and the command "**PRE?" used to read PPE.

3) Event status register (ESR) and event status enable register (ESE)

IEEE488.2 defines ESR. The command "*ESR?" may be used to read the event status register (ESR). ESE belongs to the enable part of SCPI register. If one of the bits is 1 and one of the bits in the corresponding ESR changes from 0 to 1, the ESB bit of STB should be set to 1. The command "*ESE" may be used to set ESE, and the command "*ESE?" used to read ESE.

Table 2.7 Description of event status byte

Bit	Meaning
0	Operation completed Set to this bit when the previous commands have been executed and the command *OPC has been received.
1	Not used.
2	Query error Set to this bit when the controller reads the instrument data without sending the query command, or sends a new command before reading the query data. It indicates that there is a query error, for which the query cannot be executed.
3	Instrument error Set to this bit when there is an instrument error. Error code range: -300 - -399, or positive error code. Specific error message can be found in relevant information in the error queue.
4	Execution error Set to this bit when a syntactically correct command is received but cannot be executed, and an error with code ranging from -200 to -300 is generated in the error queue.
5	Command error Set to this bit when the syntax of the command received is incorrect. Error code range: -100 - -200. Specific error message can be found in relevant information in the error queue.
6	User request Set to this bit when the instrument is switched to manual control mode.
7	Power ON Set this bit when the instrument is powered on.

4) Status: operation register

Status: The operation register contains information about the current operation of the instrument and information about the previously executed operations. The operation register value can be read by the command "STATus:OPERation:CONDition?" or "STATus:OPERation[:EVENt]?" to read the operation register value. The register is described in Table 2.8 below.

Table 2.8 Status: operation register description

Bit	Value	Definition
0	1	Unused
1	2	Channel A calibration status
2	4	Channel B calibration status (for dual-channel only)
3	8	USB interface channel calibration status
4--14	-	Unused
15	-	Always 0

5) Status: question register

The register contains instrument status that does not meet specification requirements. The register value may be queried through the command "STAT:QUES:COND" or "STAT:QUES:EVEN". The register is described in Table 2.9 below.

TIPS

Query register

Status: the question register has collected the information of all lower sub-registers (for example, bit2 has collected all time related information). Since each path corresponds to a separate sub-register, in case of a status bit error of the question register, it is required to go back to the sub-register of the path to check for the specific error source. By default, the sub-register status being queried belongs to the currently selected path.

Table 2.9 Status: question register description

Bit	Value	Definition
0--2	-	Unused
3	8	Power Summary
4--7	-	Unused
8	256	Calibration Summary
9	512	Power-on self-test
10--14	-	Unused
15	-	Always 0

2.1.5.4 Application of Status Reporting System

The status reporting system is used to monitor the status of one or more instruments in a test system. In order to correctly realize the function of the status reporting system, the controller in the test system must receive and evaluate the information of all instruments. Standard methods used include:

1) Service request (SRQ) initiated by the instrument;

2) Serial query of all instruments in the bus system, initiated by the controller in the system, in order to find the initiator of the service request and the reason.

3) Parallel query of all instruments;

4) Program command to query the status of specific instruments;

5) Query of error queue.

1) Service request

In some cases, the instrument sends a service request (SRQ) to the controller to obtain the controller's service, and the controller initiates an interrupt to enter the corresponding interrupt handler. According to Figure 2.5, an SRQ is typically initiated by one or more status bytes and by bits 2, 3, 4, 5 or 7 of the related enable register (SRE). These bits, in turn, make up advanced registers, error queues or output buffers. In order to use all the service requests as far as possible, all bits in enable registers SRE and ESE

should be set to 1.

Example: use the command *OPC to generate SRQ at the end of the sweep.

a) Recall the function InstrWrite to write the command "*ESE 1", and set to ESE bit0 (operation completed).

b) Recall the function InstrWrite to write the command "*SRE 32", and set to SRE bit5 (ESB).

c) Recall the function InstrWrite to write the command "*INIT;*OPC", and SRQ is generated after the operation is completed.

After instrument setting, the instrument generates a SRQ.

SRQ can only be initiated by the instrument. In case of an instrument error, the controller program should allow a service request to be made to the instrument and handled by a dedicated interrupt service program.

2) Serial query

Similar to the command *STB, serial query is used to query the status byte of the instrument. Serial query adopts the method of interface message, so the query speed is fast. IEEE 488.2 defines the specific method for serial query. The method is mainly used to quickly obtain the status of one or more instruments connected with the controller in the test system.

3) Parallel query

In the test system, the controller sends an information bit to the data cable through a command, and can query 8 instruments at the same time. The data configured on the data cable of the instrument is a logical "0" or "1". In addition to the conditions under which the SRE register determines the SRQ to be generated, the bits of parallel poll enable register (PPE) and STB register should be subject to AND operation. The result obtained is sent to the controller of parallel query as the response result after OR operation and NOT operation, or the result may be obtained through the command *IST.

In parallel query, first the instrument should be set to the parallel query status through the command PPC, which allocates one data cable to the instrument and determines whether the bit is reversed in response. The PPE register is used when executing parallel query. Parallel query is mainly used for the controller to quickly locate which instrument has sent the service request. Therefore, the same values should be set for the registers SRE and PPE.

4) Query instrument status

The following two commands may be used to query each part of the status register:

- Command *ESR?, *IDN?, *IST?, *STB? is used to query the advanced register;
- The status system command is used to query the SCPI register (for example: STATus:QUEStionable…).

The returned value of the register being queried is usually in decimal format and is detected by the controller program. For more details on why SRQ is generated, parallel query is usually done after SRQ.

Description of response data bit

The STB and ESR registers contain 8 bits, and the SCPI register contains 16 bits. The returned value of the query status register is in decimal format. The decimal value is equal to the sum of each bit and respective weight.

The relationship between the bit and the weight is shown in the figure below:

数据位	7	6	5	4	3	2	1	0
权 重	128	64	32	16	8	4	2	1

Figure 2.6 Relationship between the bit and the weight

5) Error queue

Each error status of the instrument corresponds to an entry in the error queue, which contains a specific error message text that can be viewed through the error log or queried through the program command: SYSTem:ERRor[:NEXT]? or SYSTem:ERRor:ALL?. If there is no error in the error queue, the query returns 0, "No error".

The error queue should be queried in the controller service request handler because a more accurate description of the cause of the error can be obtained than in the status register. Especially in the test phase of the controller program, the error queue should be frequently queried to clarify the error command record sent by the controller to the instrument.

2.1.5.5 Reset Status Reporting System

Commands and events for the reset status reporting system are listed below. In addition to the commands *RST and SYSTem:PRESet, other commands will not change the function settings of the instrument. Similarly, DCL will not change the set state of the instrument. Details are shown in the table below:

Table 2.10 Reset status reporting system

Event / Funct	Power ON/OFF (Powered status cleared)		DCL, SDC (Instrument cleared, instrument selected to be cleared)	*RST or SYSTem: PRESet	STATus: PRESet	*CLS
	0	1				
Clear STB, ESR	—	Yes	—	—	—	Yes
Clear SRE, ESE	—	Yes	—	—	—	—
Clear PPE	—	Yes	—	—	—	—
Clears the event part of the register	—	Yes	—	—	—	Yes
Clear the enable part of the operation and question registers. Fill the enable part of other registers with 1.	—	Yes	—	—	Yes	—

Event / Funct	Power ON/OFF (Powered status cleared)		DCL, SDC (Instrument cleared,	*RST or SYSTem: PRESet	STATus: PRESet	*CLS
Fill the positive transition part with 1. Clear the negative transition part.	—	Yes	—	—	Yes	—
Clear the error queue	Yes	Yes	—	—	—	Yes
Clear the output buffer	Yes	Yes	Yes	—	—	—
Clear the command processing and input buffers	Yes	Yes	Yes	—	—	—

2.1.6 Programming Precautions

1) Please initialize the instrument status before changing settings

When setting the instrument remotely, first initialize the instrument status (for example, send "*RST"), and then implement the required status setting.

2) Command sequence

In general, setting commands and query commands should be sent separately. Otherwise, the returned value of query commands will change with the current order of instrument operation.

3) Fault response

Service requests can only be initiated by the instrument. The controller program in the test system should guide the instrument to initiate service request actively when there is an error, and then enter corresponding interrupt service program for processing.

4) Error queue

Each time the controller program processes a service request, it should query the error queue of the instrument instead of the status register for a more precise cause of the error. Especially in the test phase of the controller program, the error queue should be frequently queried to obtain the error command sent by the controller to the instrument.

2.2 Instrument Program Port and Configuration

The USB program control system uses USBTMC to control the 87235.

The USBTMC interface does not require user configuration.

NOTICE

Use of USB programmable interface

Before programming with this instrument, it is necessary to install VISA library in the host computer.

2.3 I/O library

- Overview of I/O Library.....30
- Installation and Configuration of I/O Library.....31

2.3.1 Overview of I/O Library

I/O library is a pre-written software library for instruments, known as instrument driver. As a software between the computer and the instrument hardware, it consists of the function library, utility program, tool kit, etc. It is a combination of a series of software code modules and corresponds to operation of a plan, such as configuring the instrument, reading from the instrument, writing to the instrument and triggering the instrument, etc. Residing in the computer, it is the bridge and link between the computer and the instrument. By providing a high-level modular library for convenient programming, users no longer need to learn the complex low-level programming protocol for a specific instrument. Application of instrument driver is the key to develop test and measurement applications quickly.

Functionally, a universal instrument driver generally consists of five parts: functor, interactive developer interface, programmer interface, subprogram interface and I/O interface, as shown in the figure below:

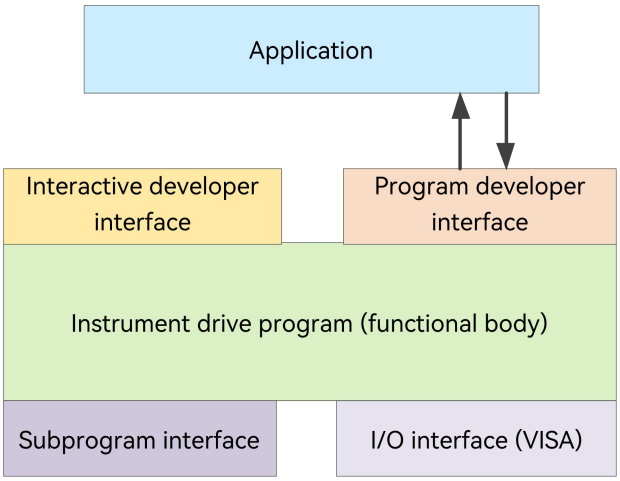


Figure 2.7 Structure model of instrument driver

The details are as follows:

1) Functor. As the main function part of the instrument driver, it may be understood as its framework program.

2) Interactive developer interface. Application development environment that supports instrument driver development is usually provided with graphical interactive developer interface for user convenience. For example, in Labwindows/CVI, the function panel is an interactive developer interface. In the function panel, each parameter of the instrument driver function is represented as a graphical control.

3) Programmer interface. It is a software interface for the application to recall instrument driver function, such as dynamic link library file.dll of instrument driver in Windows system.

4) I/O interface. It completes the actual communication between the instrument driver and the instrument. The bus specific I/O software, such as GPIB and RS-232, or the common standard I/O software used across multiple buses, VISA I/O, may be used.

5) Subprogram interface. It is a software interface for the instrument driver to access other support libraries, such as databases, FFT functions, etc. The subprogram interface is used when the instrument driver needs to recall other software modules, operating systems, program code libraries and analysis function libraries to complete its task.

2.3.2 Installation and Configuration of I/O Library

Along with the application in test field, it has gone through different development stages from traditional instrument to virtual instrument. In order to solve the interchangeability of instruments and reusability of test program in automatic test system, instrument driver has gone through different development processes. IVI (Interchangeable Virtual Instruments) driver is relative popular and common at present. Based on IVI specification, it defines a new instrument programming interface, inserts the class driver and VPP architecture onto the VISA to make the test application and instrument hardware completely independent, adds such unique functions as instrument simulation, range sensing and status cache, improves the operation efficiency of the system, and realizes instrument exchange.

There are two types of IVI driver: IVI-C and IVI-COM, where the latter adopts the form of COM API based on the component object model (COM) of Microsoft, and the former adopts the form of C API based on ANSI C. Both types are designed according to the instrument class defined in the IVI specification and have the same application development environment, including Visual Studio, Visual Basic, Keysight VEE, LabVIEW, CVI/LabWindows, etc.

TIPS

Port configuration and IO library installation

Before using the computer to control the 87235, please make sure you have the necessary ports and I/O libraries installed and configured correctly.

TIPS

Use of I/O library

The driver function panel, help document and driver function examples will be installed automatically when installing the attached IVI-COM/C driver installation package, so as to facilitate users to develop integrated program functions.

2.4. Zeroing

- InternalZeroing.....31
- ExternalZeroing.....31

Zeroing is used to deduct channel noise. When should zeroing be carried out? It is recommended that the 87235 be zeroed in the following cases:

- When the temperature change exceeds 5℃;
- After the connection is established with the device under test;
- Shutdown and reboot;

- After 24 hours;
- Before measuring the low-power signal. For example, when measuring a signal 20dB higher than the minimum power specified in the 87235.

Related program control commands:

CALibration:ZERO:AUTO

CALibration:ZERO:TYPE

2.4.1 Internal zeroing

The 87235 can be internally zeroed through the instrument switch control, so there is no need to disconnect the Power Sensor from the device under test or turn off the output signal of the device under test during use, which can speed up the measurement, reduce connector wear, and lower the measurement uncertainty.

For example, if configured for internal zeroing and zeroing is initiated once:

CALibration:ZERO:TYPE INT

CAL:ZERO:AUTO ONCE

For example, if configured to "Allow auto-zero" status:

CAL:ZERO:AUTO ON

For example, if configured to "Disable auto-zero" status:

CAL:ZERO:AUTO OFF

2.4.2 External zeroing

In the average mode, signals as low as -70dBm can be measured, when the output of the device under test needs to be turned off and external zeroing is performed.

For example, zeroing:

CALibration:ZERO:TYPE EXT

CAL:ZERO:AUTO ONCE

2.5 Performing Measurements

The measurement can be configured as absolute power measurement, differential power measurement, ratio power measurement, relative power measurement, etc. For details, refer to "3.3.3 Measurement Subsystem Commands".

2.6 Using Frequency Response Offset Table

- Overview.....33
- Enter Frequency Offset Table.....33
- Select Frequency Offset Table.....34
- Enable Frequency Offset Table.....34
- Measurement Applications.....34
- Specific Applications.....34

How to use the frequency response offset (hereinafter referred to as frequency offset) table? The frequency offset table is used to compensate the frequency response in the

process of measurement establishment.

2.6.1 Overview

Enable or disable the frequency offset table with [SENSe[1]:]CORRection:CSET2:STATe. When enabled, the frequency offset table provides a quick way to compensate for the frequency response in the test system. It should be noted that when enabled, the frequency offset is an "additional" frequency response to 87235, that is, the inherent frequency response of the 87235 (stored in the EEPROM of the 87235) is also taken into account. The 87235 can store up to 10 frequency offset tables, each with up to 80 frequency points.

How to use the frequency offset table:

a) Enter Frequency Offset Table

b) Select Frequency Offset Table

c) Enable Frequency Offset Table

d) Measurement Applications

2.6.2 Input Frequency Offset Table

a) Entry steps

- Enter the frequency list: MEMory:TABle:FREQuency <frequency 1>{, <frequency i>}. such as 50 MHz, 1 GHz, 10 GHz, 40 GHz;
- Enter the offset factor corresponding to the frequency list: MEMory:TABle:GAIN <factor 1>{, <factor i>}. For example, 100, 98.8, 101.2, and 110.8 correspond to the offset factors of 50 MHz, 1 GHz, 10 GHz and 40 GHz, respectively;
- Rename the frequency offset table if necessary: MEMory:TABLe:MOVE <original name>, <target name>. For example "User_3", "MyFdo0"

b) Enumerate the name of the frequency offset table: MEMory:CATalog:TABLe? See the description of this command for more information.

c) Rename the frequency offset table: MEMory:TABLe:MOVE <original name>, <target name>.

d) Query the data in the frequency offset table. For example, query the data in the frequency offset table with sequence number 3.

- Query the frequency points in the frequency offset table: MEMory:TABLe3:FREQuency:POINTs?
- Query the frequency list in the frequency offset table: MEMory:TABLe3:FREQuency?
- Query the number of factor points in the frequency offset table: MEMory:TABLe3:GAIN[:MAGNitude]:POINTs?
- Query the factor list in the frequency offset table: MEMory:TABLe3:GAIN[:MAGNitude]?

e) Modify the data in the frequency offset table: see a).

f) Notes

- The frequency list is arranged in ascending order;
- The effective suffix of the frequency list is Hz, kHz, MHz and GHz. Hz by default;

- Ensure that the frequency list is within the effective frequency range of the 87235;
- The name of the frequency offset table is up to 12 bytes and no spaces are allowed.

2.6.3 Select Frequency Offset Table

[SENSe[1]:]CORRection:CSET2[:SELect] <frequency offset table name>, e.g. "User_3"

2.6.4 Enable Frequency Offset Table

[SENSe[1]:]CORRection:CSET2:STATe ON

2.6.5 Measurement Applications

- ABOR
- CONF:POW:AC DEF,1,(@1)
- SENS:CORR:CSET2:SEL "MyFdo0"
- SENS:CORR:CSET2:STAT ON
- SENS:FREQ 5GHz
- INIT1
- FETC?

2.6.6 Specific Applications

a) Suppose the frequency list of frequency offset table is: 500MHz, 1GHz, 11GHz. The list of offset factors is: 100, 10, 10. Let the signal frequency be Freq and the calculated offset factor be Gain.

b) If Freq is outside the range of the frequency offset table, the frequency bias value of the highest or lowest frequency point in the frequency offset table is used. For example, for 18 GHz, the offset factor 102 corresponding to the maximum frequency point of 10 GHz is used. For example, for 50MHz, the offset factor 100 corresponding to the minimum frequency point of 500MHz is used.

c) If Freq is within the valid range of the frequency list, but between two frequencies (Freq1, Freq2), such as 5 GHz, the offset factor is obtained using two-point linear interpolation, and the offset factors corresponding to Freq1 and Freq2 are set to Gain1 and Gain2, respectively. Gain is calculated to be 50 by the following equation.

$$Gain = Gain1 + \frac{Freq - Freq1}{Freq2 - Freq1} \times (Gain2 - Gain1)$$

d) If the power before using the frequency offset table is 1.000mW (noted as Pwr0), and the final displayed power is Pwr, then Pwr = Pwr0/Gain/100 = 2.000mW.

2.7 Setting Display Resolution

Related program control commands:

DISPlay[:WINDow[1]|2][:NUMeric[1]|2]:RESolution <resolution>

< Resolution> ranges from 1 to 4.

For linear power display, <resolution> represents the number of valid digits displayed; for logarithmic power display, <resolution> represents the number of digits after the decimal point.

2.8 Setting Average

2.8.1 Measurement Average

The 87235 memory has a digital filter for average power readings. The average times ranges from 1 to 1024. If the average state is turned on, the measurement time will be increased.

Set to auto-average state, that is, set different averaging times according to different power level and display resolution. Generally, the lower the power, the greater the average times; the higher the resolution, the larger the average times.

Related program control commands:

[SENSe[1]:]AVERage[:STATe] <switch> Set average switch

For example, turn on the measurement average switch:

SENS:AVER 1

Turn off the Measurement Average.

AVER 0

[SENSe[1]:]AVERage:COUNt:AUTO <switch> Set auto-average switch

[SENSe[1]:]AVERage:COUNt <average times> Set average times

2.8.2 Video Average

Video average, also known as trace average, is used to reduce the effect of noise on the traces. The average times ranges from 1 to 1024. If the video average state is turned on, the measurement time will be increased.

Related program control commands:

[SENSe[1]:]AVERage2[:STATe] <average switch> Set average switch

For example, turn on the video average switch:

SENS:AVER2 1

Turn on the Video Average:

AVER2 0

2.9 Setting Offset

The 87235 can compensate for signal attenuation or gain in test equipment (e.g., compensate for a 20 dB attenuator).

Related program control commands:

[SENSe[1]:]CORRection:GAIN2 <offset value> Set channel offset value

[SENSe[1]:]CORRection:GAIN2:STATe <switch> Set channel offset switch

For example, set the channel offset to 3dB.

SENS:CORR:GAIN2 3

2.10 Setting Measurement Limits

Verify that the measured power is not outside the given range by setting the

measurement limits.

Related program control commands:

:CALCulate[1]|2|3|4:LIMit:LOWer[:DATA] <lower limit> Set lower limit

:CALCulate[1]|2|3|4:LIMit:UPPer[:DATA] <upper limit> Set upper limit

:CALCulate[1]|2|3|4:LIMit:STATe <switch> Set limit detection switch

:CALCulate[1]|2|3|4:LIMit:FAIL? Query whether the limit is exceeded

:CALCulate[1]|2|3|4:LIMit:FCOunt? Number of times to query whether the limit is exceeded (FCO)

:CALCulate[1]|2|3|4:LIMit:CLEar[:IMMediate] Clear the failure count (FCO).

2.11 Status Report

The status report is used to detect the error information, operation status, question status, etc. of the power. The status report adopts the principle of step-by-step reporting, such as calibration operation is reported to operation status, and operation status is reported to status word.

For example, query whether the instrument is being calibrated, whether the instrument is being finished calibrating, whether there is an error in zero calibration, whether the instrument is connected to 87235, whether zero calibration is required, and whether the measurement is out of range, etc. The following is a description of "querying whether the instrument is calibrating Channel A".

Bit 1 in the register group of STATus:OPERation:CALibrating indicates the calibration status of Channel A.

Set the event occurrence of the calibration operation to detect the event when there is a transition from uncalibrated (state 0) to calibrated (state 1), i.e., set the positive transition filter to 1.

STAT:OPER:CAL:PTR 2(Configure the calibration event detection for Channel A to be from 0 to 1) Note 1

Report calibration operation events to its higher-level operation status register. That is, the calibration status bit (bit 0) of the STATus:OPERation register group.

STAT:OPER:CAL:ENAB 2 (The parameter can be 4, or 6 if it is necessary to report events for Channel B). Note 1

Similarly, if it is necessary to further report the operation status to bit 7 of the "status word", set the corresponding bit (bit 0) of the operation positive transition filter and the corresponding bit (bit 0) of the enable register.

STAT:OPER:CAL:PTR 1(Configure the calibration event detection to be from 0 to 1)

STAT:OPER:ENAB 1 (The parameter can be 2048, or 2049 if the lower detection event needs to be reported).

At this point, the configuration is complete, and the next step is to query whether Channel A is being calibrated.

Method 1: Query bit 1 of the calibration operation condition register. If it returns non-zero, it indicates that it is being calibrated.

STAT:OPER:CAL:COND?

Method 2: Query bit 0 of the operation condition register. If it returns non-zero, it indicates that it is being calibrated.

STAT:OPER:COND?

Method 3: Query bit 7 of the status word. If it returns non-zero, it indicates that it is being calibrated.

*STB?

Note 1: If it is necessary to query whether one of the two channels is being calibrated, change parameter 2 to 6 (bit 1 and bit 2 indicate Channel A and Channel B, respectively).

2.12 Storing/Recalling

To reduce repetitive setup processes, the instrument can store 10 types of configuration data into non-volatile memory. Error list, program-controlled address (such as IP address, instrument string number), frequency response offset table, zero calibration information, etc. are not stored in this configuration. Except for the error list, which is not stored, everything else is stored in the hard configuration file and does not change with user calls.

Related program control commands:

*SAV <NRf>

*RCL <NRf>

<NRf> ranges from 1 to 10.

3. Program Control Commands

- Description of Commands.....39
- Common Commands.....39
- Instrument Subsystem Commands.....46

3.1 Description of Commands

This section provides detailed command reference information for remote control, including:

- Complete syntax format and parameter list;
- Syntax diagram for non-standard SCPI;
- Detailed function description and related command description;
- Supported command formats (settings or queries);
- Parameter description, including: data type, value range and default value (unit);
- Key path;
- Model of instrument in the same class of instrument that is compatible with the command. If not specified, it indicates that the current command only applies to this series.
- Other instructions.

The sections of common commands and instrument subsystem commands first list the order of command items to make convenient for users to query.

For remote control, the following table describes the command suffixes:

Table 3.1 Description of command suffixes

Suffixes	Value range	Description
<ch>	1..1	Channel
<m>	1..4	Measure
<t>	1..10	Frequency response offset table

3.2 General Commands(IEEE488.2 Commands)

Common commands are used to control instrument status registers, status reports, synchronization, data storage and other common functions. The use and function of common commands apply to different instruments. All common commands may be identified by the first "*" in the command word, and are defined in detail in IEEE488.2.

IEEE488.2 common command is interpreted and explained below.

- *CLS.....40
- *DDT.....40
- *ESE.....40
- *ESR?.....42
- *IDN?.....42

3.2 General Commands(IEEE488.2 Commands)

- *OPC....42
- *OPT....42
- *RCL....43
- *RST....43
- *SAV....43
- *SRE....43
- *STB?....44
- *TRG....45
- *TST?....45
- *WAI....45

TIPS

Command use:
Unless otherwise specified, commands may be used for setting or query.
If a command is used only for setting or querying, or to start an event, the command description will be explained separately.

*CLS

Function:	Clear the instrument status data structure, including SCPI registers (such as question status, operation status, etc.), standard event registers, status words, and error/event queues.	
Query:	Not supported	
Setting:	*CLS	
Example:	*CLS	Clear the instrument status
Error message:	None	
Reset state:	None	

*DDT

Function:	Query or set the operation in response to *TRG general command. Note: The 87235 does not support this command at the moment. This command is used for expansion.
Query:	*DDT?
Setting:	*DDT <Arbitrary data block> | <string> Arbitrary data block is of the form: #nN<action> The string will be of the form "<action>" 1) Action has the following forms: FETC? FETC1?

FETC2?

*TRG

TRIG1

TRIG2 (for dual-channel Power Sensor only)

2) In arbitrary data block, the first value n after # represents the number of bits of the data length, and the next value represents the length of the data block.

Example: #15FETC? -- n = 1, N = 5 (5 bytes in total for FETC?)

Example: *DDT? Query the operation behavior of the instrument when it receives the *TRG command.

*DDT #206FETCh?

*DDT "FETCh?"

*DDT "TRIG1;FETC1"

Error message: None

Reset state: None

*ESE

Function: Query or set the standard event status enable register. 0 for disable, and 1 for enable.

Query: *ESE?

Setting: *ESE <NRf>

NRf denotes the numerical value, a multiple of 2. See Table 3.2 for bit mapping.

Example: *ESE? Query the current setting of this register. The return format is <NR1>, 0-255.

*ESE 60 Enable 4+8+16+32 corresponding bits.

Table 3.2 Standard event bit mapping

Bit	Value	Description
0	1	Operation completed
1	2	Unused
2	4	Query error
3	8	Device-related errors
4	16	Execution error
5	32	Command error
6	64	Unused
7	128	Unused

3.2 General Commands(IEEE488.2 Commands)

*ESR?

Function:	Query the value of the standard event state register and clear the register. Refer to Table 3.2	
Query:	*ESR?	
Setting:	Not supported	
Example:	*ESR?	Query the value of the standard event state register and clear it.
Error message:	None	
Reset state:	None	

*IDN?

Function:	Query the identification string of 87235. Related program control commands ":SYSTem:IDN", ":SYSTem:IDN:AUTO" If ":SYSTem:IDN:AUTO" is set to "ON", *IDN? returns the user string defined by ":SYSTem:IDN", otherwise returns the string preset by the 87235.	
Query:	*IDN?	
Setting:	Not supported	
Example:	*IDN?	Return the string preset by the 87235.
Error message:	None	
Reset state:	None	

*OPC

Function:	When all waiting operations are completed, set the operation end bit in the standard event state register.	
Query:	*OPC?	
Setting:	*OPC	
Example:	*OPC?	Return 1 if the waiting operation completes, otherwise it waits.
Error message:	None	
Reset state:	None	

*ESE?

Function:	Query the instrument option configuration.
Query:	*ESE?
Setting:	Not supported
Example:	*ESE?

Error message: None

Reset state: None

*RCL

Function: Call the 87235 status in the specified storage call register.

Query: Not supported

Setting: *RCL <NRf>
The range is from 1 to 10

Example: *RCL 8

Error message: If the registers are not located from 1 to 10, it prompts "-222, "Data out of range"".

Reset state: None

*RST

Function: To reset 87235, please refer to SYSTem:PRESet.

Query: Not supported

Setting: *RST

Example: *RST

Error message: None

Reset state: None

*SAV

Function: Store the instrument status into the specified register.

Query: Not supported

Setting: *SAV <NRf>
The range is from 1 to 10

Example: *SAV 9

Error message: If the registers are not located from 1 to 10, it prompts "-222, "Data out of range"".

Reset state: None

*SRE

Function: Query or set the service request register 0 for disable, and 1 for enable.

Query: *SRE?

Setting: *SRE <NRf>
NRf denotes the numerical value, a multiple of 2. See Table 3.3 for bit

mapping.

Example: *SRE? Query the current setting of this register. The return format is <NR1>, 0-255.

*SRE 188 Set bits 2, 3, 4, 5 and 7 respectively (4+8+16+32+128).

Error message: None

Reset state: None

Table 3.3 Service request register bit mapping

Bit	Value	Description
0	1	Unused
1	2	Device information
2	4	Error/event queue
3	8	Question status
4	16	Information reception
5	32	Event status bit
6	64	Must be 0
7	128	Operation status

*STB?

Function: Query the status word.

Query: *STB?

Setting: Not supported

Example: *STB?

Error message: None

Reset state: None

Bit mapping is as follows:

Table 3.4 Status word

Bit	Value	Description
0	1	Unused
1	2	Device information
2	4	Error/event queue
3	8	Question status
4	16	Information reception
5	32	Event status bit

6	64	Service request
7	128	Operation status

*TRG

Function: Trigger all channels in Wait for Trigger. The function of *TRG can be changed with *DDT.

Query: Not supported

Setting: *TRG

Example: *TRG

Error message: If the trigger source is not BUS, it prompts "-211, "Trigger ignored"".

Reset state: None

*TST?

Function: Execute self-test with longer self-test time.

Query: *TST?

Setting: Not supported

Example: *TST? Returning 0 means pass, and 1 means fail.

Error message: None

Reset state: None

*WAI

Function: Place 87235 in a wait state until either of the following is satisfied:
All waiting operations have been completed
Device clear command received
Restart.

Query: Not supported

Setting: *WAI

Example: *WAI

Error message: None

Reset state: None

3.3 Instrument Subsystem Command

This section details the subsystem commands of the 87235.

- Calculation Subsystem Command (CALCulate)....46
- Calibration Sub-system Command (CALibration)....53
- Measurement Subsystem Command (CONFigure/FETCh/READ/MEASure) 56
- Display Subsystem Command (DISPlay)....65
- Format Subsystem Command (FORMat)....66
- Memory Subsystem Command (MEMory/MMEMory)....67
- Sensor Subsystem Command (SENSe)....73
- Status Subsystem Command (STATus)....89
- System Subsystem Command (SYSTem)....128
- Trigger Subsystem Command (INITiate/ TRIGger)....143
- Unit Subsystem Command (UNIT)....143
- Service Subsystem Command (SERVice)....151

3.3.1 Calculation Subsystem Command (CALCulate)

The calculation (CALCulate) subsystem is used for subsequent data processing and shares four independent calculation function blocks that correspond to measurements as follows:

CALC1 (Measurement 1)
CALC2 (Measurement 2)
CALC3 (Measurement 3)
CALC4 (Measurement 4)

Figure 3.1 Correspondence between CALC and measurement

Both sensing (SENSe) subsystems can be used as inputs to the calculation subsystem (FEED), and the calculation diagram is as follows:

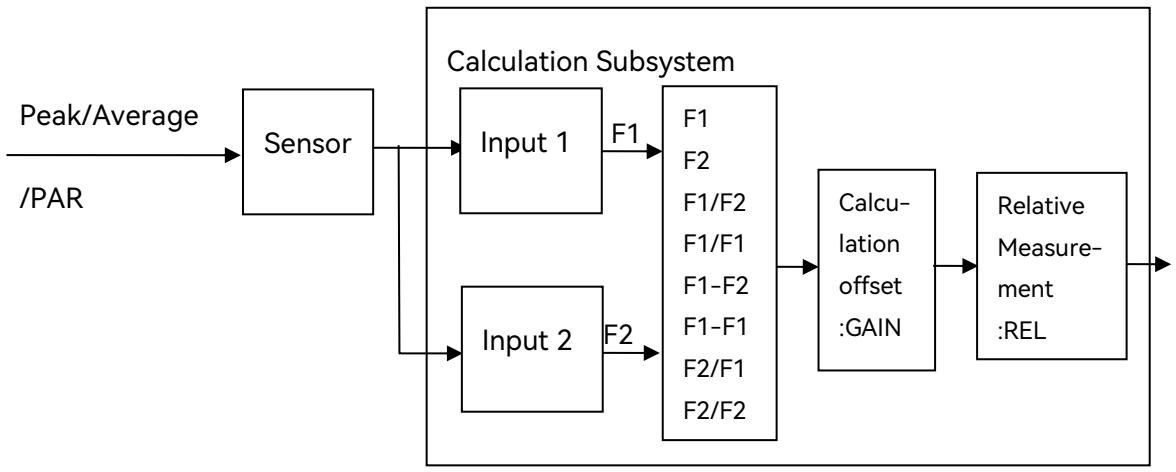


Figure 3.2 Calculation diagram

The calculation offset and relative measurement are calculated when the switch is turned on.

Commands include:

- :CALCulate[1]|2|3|4:FEED[1]|2.....47
- :CALCulate[1]|2-4:GAIN[:MAGNitude].....48
- :CALCulate[1]|2|3|4:GAIN:STATe.....48
- :CALCulate[1]|2|3|4:LIMit:CLEar:AUTO.....49
- :CALCulate[1]|2|3|4:LIMit:CLEar[:IMMediate].....49
- :CALCulate[1]|2|3|4:LIMit:FAIL?.....49
- :CALCulate[1]|2|3|4:LIMit:FCOunt?.....50
- :CALCulate[1]|2|3|4:LIMit:LOWer[:DATA].....50
- :CALCulate[1]|2|3|4:LIMit:STATe.....51
- :CALCulate[1]|2|3|4:LIMit:UPPer[:DATA].....52
- :CALCulate[1]|2|3|4:MATH[:EXPRession].....52
- :CALCulate[1]|2|3|4:MATH[:EXPRession]:CATalogue?.....53
- :CALCulate[1]|2|3|4:RELative[:MAGNitude]:AUTO.....53
- :CALCulate[1]|2|3|4:RELative[:MAGNitude]:VALue?.....54
- :CALCulate[1]|2|3|4:RELative:STATe.....54

:CALCulate[1]|2|3|4:FEED[1]|2

Function: Query or set the measurement mode. The CALC:MATH:EXPR command is used to determine it from which channel.

The meaning of the suffixes in CALC: 1 for Measurement 1, 2 for Measurement 2, 3 for Measurement 3, and 4 for Measurement 4. The same below.

Query: :CALCulate[1]|2|3|4:FEED[1]|2?

Setting: :CALCulate[1]|2|3|4:FEED[1]|2 <string>

Parameters in the form of "POW:PEAK", "POW:PTAV", "POW:AVER", "POW:MIN"

Alternatively, it can be followed by ON SWEEP[1]|2|3|4 to indicate which measurement gate it is. For example, "POW:AVER ON SWEEP3" means the average power in measurement gate 3. If ON SWEEP[1]|2|3|4 is not specified, the measurement gate remains unchanged.

Input 2 (FEED2) is used only for ratio measurements and difference measurements.

Example:

CALC2:FEED?	Query the measurement mode of Input 1 of Measurement 2.
CALC:FEED2 "POW:AVER ON SWEEP3"	Set Input 2 of Measurement 1 to the average power in measurement

gate 3.

Error message: If the mode contains ON SWEEP[1]|2|3|4, but the trigger source is not EXT or INT, it prompts "-221, "Settings conflict"".

Reset state: None.

:CALCulate[1]|2|3|4:GAIN[:MAGNitude]

Function: Query or set the calculation offset value of the specified measurement, in DB and in the range of -100 to 100. After successful setup, the calculation offset switch for this measurement is automatically turned on.

The related command is :CALCulate[1]|2|3|4:GAIN:STATe, which is used to set or query the calculation offset switch.

Query: :CALCulate[1]|2|3|4:GAIN[:MAGNitude]? [MIN|MAX]

Setting: :CALCulate[1]|2|3|4:GAIN[:MAGNitude] <numeric data>

The form of <numeric data>: DEF, MIN, MAX, and NRf, where DEF is only used for setting.

DEF means 0dB, MIN means -100dB, and MAX means 100dB

Example:

CALC:GAIN?	Query the calculation offset of Measurement 1.
CALC2:GAIN? MIN	Query the minimum value of the settable calculation offset of Measurement 2.
CALC3:GAIN MAX	Set the calculation offset of Measurement 3 to the maximum value.
CALC4:GAIN 18	Set the calculation offset of measurement 4 to 18 dB.

Error message: None

Reset state: Set to 0 (DEF).

:CALCulate[1]|2|3|4:GAIN:STATe

Function: Query or set the switch state of the calculation offset in the specified measurement.

The related command is :CALCulate[1]|2|3|4:GAIN[:MAGNitude], which is used to set or query the operation value.

Query: :CALCulate[1]|2|3|4:GAIN:STATe?

Setting: :CALCulate[1]|2|3|4:GAIN:STATe <Boolean data>

Valid forms of <Boolean data> are: 0, OFF, 1, ON

Example:

CALC:GAIN:STAT?	Query the calculation offset switch state of Measurement 1.
CALC2:GAIN:STAT ON	Enable the calculation offset of Measurement 2.
CALC3:GAIN:STAT 0	Disable the calculation offset of Measurement 3.

Error message	None
Reset state:	Off

:CALCulate[1]|2|3|4:LIMit:CLEar:AUTO

Function:	Control when the limit FCO (failure count) is cleared.
Query:	:CALCulate[1]|2|3|4:LIMit:CLEar:AUTO? For the ONCE state, return 1 if no measurement is not started, otherwise return 0 For the OFF state, always return 0 For the ON state, return 1 if the measurement is started, otherwise return 0
Setting:	:CALCulate[1]|2|3|4:LIMit:CLEar:AUTO <Boolean data>|ONCE|2 Valid forms of <Boolean data> are: 0, OFF, 1, ON. For "ON", the FCO is set to 0 when the following operations are performed: Initialize with the INITiate[:IMMediate] command; Initialize with the INITiate:CONTinuous ON command; Measure with the MEASure? command; Read the measurement with the READ? command. For "OFF", FCO is not cleared. For "ONCE" or 2, it is only cleared at the first initialization and then accrued when a limit detection failure is encountered.
Example:	CALC1:LIM:CLE:AUTO? — Query FCO clear state of Measurement 1. CALC2:LIM:CLE:AUTO ONCE — Set the FCO for clearing Measurement 2 on the first initialization.
Error message	None
Reset state:	Set to ON.

:CALCulate[1]|2|3|4:LIMit:CLEar[:IMMediate]

Function:	Clear the FCO (failure count) of the specified measurement, which can be queried by CALCulate[1]|2|3|4:LIMit:FCOunt?.
Query:	Not supported
Setting:	:CALCulate[1]|2|3|4:LIMit:CLEar[:IMMediate]
Example:	:CALC:LIM:CLE — Clear the failure count of Measurement 1.
Error message	None
Reset state:	None.

:CALCulate[1]|2|3|4:LIMit:FAIL?

Function:	Query whether the specified measurement exceeds the limit. 1 means Yes, 0

means No.

Query: :CALCulate[1]|2|3|4:LIMit:FAIL?

Setting: Not supported

Example: :CALC:LIM:FAIL? Query the detection state of Measurement 1.

Error message: None

Reset state: None

:CALCulate[1]|2|3|4:LIMit:FCOunt?

Function: Query the limit detection failure count (FCO) of the specified measurement.
The FCO is cleared in the following cases:
a) Reset
b) CALCulate[1]|2|3|4:LIMit:CLEar:IMMediate
c) CALCulate[1]|2|3|4:LIMit:CLEar:AUTO ON

Query: Query: :CALCulate[1]|2|3|4:LIMit:FCOunt?

Setting: Not supported

Example: :CALC:LIM:FCO? Query the detection failure count of Measurement 1.

Error message: None

Reset state: None

:CALCulate[1]|2|3|4:LIMit:LOWer[:DATA]

Function: Query or set the lower limit of the specified measurement limit.

Query: :CALCulate[1]|2|3|4:LIMit:LOWer[:DATA]? [MIN|MAX]

Setting: :CALCulate[1]|2|3|4:LIMit:LOWer[:DATA] <numeric data>
The form of <numeric data>: DEF, MIN, MAX, and NRf, where DEF is only used for setting.
If the currently set lower limit value is more than or equal to the upper limit value, the upper limit value is automatically adjusted depending on the unit, as shown in Table 3.7.

Example: CALC:LIM:LOW? Query the lower limit of Measurement 1.

CALC4:LIM:LOW 0.2 According to the display unit of measurement, set the lower limit of measurement 4 as:
0.2dBm at dBm
200mW at W
0.2dB at dB
0.2% at %.

Error: None

message

Reset state: All measurements are set to -90dBm or -90dB.

Table 3.5 Unit of measurement

Measurement mode	Measurement type	CALC:REL:STAT OFF		CALC:REL:STAT ON	
		Linear	Logarithm	Linear	Logarithm
Single channel	Peak, average	Watt	dBm	%	dB
	Peak-to-average ratio	%	dB	%	dB
Ratio	Average, peak, peak-to-average ratio	%	dB	%	dB
Delta	Peak, average	Watt	dBm	%	dB
	Peak-to-average ratio	%	dB	%	dB

Table 3.6 Limit range

	Watt	dBm	%	dB
DEF	1pW	-90	100p%	-120
MIN	1aW	-150	100a%	-180
MAX	1XW	200	100X%	180

Table 3.7 Limit range adjustment

Lower limit value	Upper limit value			
	Watt	dBm	%	dB
$nLow$	$nLow \times 10^{0.001}$	$nLow + 0.01$	$nLow \times 10^{0.001}$	$nLow + 0.01$

:CALCulate[1]|2|3|4:LIMit:STATe

Function: Query or set the specified measurement limit detection switch.

Query: :CALCulate[1]|2|3|4:LIMit:STATe?

Setting: :CALCulate[1]|2|3|4:LIMit:STATe <Boolean data>
Valid forms of <Boolean data> are: 0, OFF, 1, ON

Example:

CALC:LIM:STAT?	Query the limit detection switch state of Measurement 1.
CALC2:LIM:STAT ON	Enable the limit detection of Measurement 2.
CALC3:LIM:STAT 0	Disable the limit detection of Measurement 3.

Limit: When the [SENSe[1]:]MRATe command is set to FAST mode, the limit measurement is disabled, but the setting is allowed, and the setting takes effect

after exiting this measurement mode.

Error message: None

Reset state: Disable the measurement limit detection.

:CALCulate[1]|2|3|4:LIMit:UPPer[:DATA]

Function: Query or set the upper limit of the specified measurement limit. Refer to CALCulate[1]|2|3|4:LIMit:LOWer[:DATA]

Query: :CALCulate[1]|2|3|4:LIMit:UPPer[:DATA]? [MIN|MAX]

Setting: :CALCulate[1]|2|3|4:LIMit:UPPer[:DATA] <numeric data>

The form of <numeric data>: DEF, MIN, MAX, and NRf, where DEF is only used for setting.

If the currently set upper limit value is less than or equal to the lower limit value, the lower limit value is automatically adjusted depending on the unit, as shown in Table 3.9.

Example:

CALC:LIM:UPP?	Query the lower limit of Measurement 1.
CALC4:LIM:UPP 8	According to the display unit of measurement, set the upper limit of measurement 4 as: 8dBm at dBm 8W at W 8dB at dB 8% at %.

Error message None

Reset state: All measurements are set to 90dBm or 90dB.

Table 3.8 Limit range

	Watt	dBm	%	dB
DEF	1MW	90	100M%	60
MIN	1aW	-150	100a%	-180
MAX	1XW	200	100X%	180

Table 3.9 Limit range adjustment

Upper limit value	Lower limit value			
	Watt	dBm	%	dB
$nUpp$	$nUpp/10^{0.001}$	$nUpp-0.01$	$nUpp/10^{0.001}$	$nUpp-0.01$

:CALCulate[1]|2|3|4:MATH[:EXPRession]

Function: Query or set the expression of the specified measurement: single channel, difference and ratio

Query: :CALCulate[1]|2|3|4:MATH[:EXPRession]?

Setting: :CALCulate[1]|2|3|4:MATH[:EXPRession] <string>

The form of string is as follows:

For a single-channel Power Sensor, such as the 87235:

"(SENS1)", "(SENS1-SENS1)", "(SENS1/SENS1)"

For a dual-channel Power Sensor, such as the 2438:

"(SENS1)", "(SENS2)",

"(SENS1-SENS1)", "(SENS2-SENS2)",

"(SENS1-SENS2)", "(SENS2-SENS1)",

"(SENS1/SENS1)", "(SENS2/SENS2)",

"(SENS1/SENS2)", "(SENS2/SENS1)",

Example:

CALC1:MATH?	Query the measurement expression of Measurement 1.
CALC2:MATH "(SENS1/SENS1)"	Set the expression of Measurement 2 to the Channel A/B ratio measurement.

Error message None

Reset state: Set to Channel A ("(SENS1)").

:CALCulate[1]|2|3|4:MATH[:EXPRession]:CATalogue?

Function: Enumerate all measurement expressions, separated by commas.

For a single-channel Power Sensor, the string is:

"(SENS1)", "(SENS1-SENS1)", "(SENS1/SENS1)"

For a dual-channel Power Sensor, the string is:

"(SENS1)", "(SENS2)", "(SENS1/SENS2)", "(SENS2/SENS1)",

"(SENS1-SENS2)", "(SENS2-SENS1)""(SENS1-SENS1)",

"(SENS2-SENS2)", "(SENS1/SENS1)", "(SENS2/SENS2)"

Query: :CALCulate[1]|2|3|4:MATH[:EXPRession]:CATalogue?

Setting: Not supported

Example:

CALC:MATH:CAT?	List all defined mathematical expressions.

Error message: None

Reset state: None

:CALCulate[1]|2|3|4:RELative[:MAGNitude]:AUTO

Function: Set the reference value for relative measurement. In the CALCulate block, the relative value is used for the measured signal only after any mathematical computation and calculation offset are completed. This value should be set

to ONCE to set the reference value for relative measurement. After setting the reference value, the command returns OFF. Set the command to ONCE to set the command

CALCulate[1]|2|3|4:RELative:STATe is transformed to ON.

0|OFF does not perform any operation.

1|ON is invalid, 87235 returns an error: invalid parameter.

2|ONCE, valid parameter. Refer to the above for meaning.

Query: :CALCulate[1]|2|3|4:RELative[:MAGNitude]:AUTO?

Setting: :CALCulate[1]|2|3|4:RELative[:MAGNitude]:AUTO ONCE

Example: CALC:REL:AUTO? Always return 0.

CALC:REL:AUTO ONCE Set the reference value for the relative measurement of Measurement 1.

Error message: If parameter 1 or ON is selected, it prompts "-224, "Illegal parameter value"".

Reset state: None

:CALCulate[1]|2|3|4:RELative[:MAGNitude]:VALue?

Function: Query the reference value for relative measurement.

Query: :CALCulate[1]|2|3|4:RELative[:MAGNitude]:VALue?

Setting: Not supported

Example: CALC:REL:VAL? Query the reference value for the relative measurement of Measurement 1.

Error message: None

Reset state: None

:CALCulate[1]|2|3|4:RELative:STATe

Function: Query or set the relative measurement switch status.

When turned on, the relative measurement value set by :CALCulate[1]|2|3|4:RELative[:MAGNitude]:AUTO is applied to the measurement.

Query: :CALCulate[1]|2|3|4:RELative:STATe?

Setting: :CALCulate[1]|2|3|4:RELative:STATe<Boolean data>

Example: CALC:REL:STAT? Return 1 when the relative measurement of Measurement 1 is ON, otherwise return 0.

CALC2:REL:STAT ON Turn on the relative measurement status of Measurement 2.

Error message: None

Reset state: Disable relative measurement.

3.3.2 Calibration Sub-system Command (CALibration)

The CALibration subsystem is used to control the automatic zero bias setting and linearity adjustment of the 87235. If there is no RF signal loaded to the 87235, the zero calibration setting can be done at any time.

The numeric suffix in CALibration command indicates the measurement channel. CALibration1 and CALibration2 indicate Channel A and Channel B respectively (the 87235 series only supports Channel A.)

Commands include:

- :CALibration[1][:ALL]……55
- :CALibration[1]:AUTO……55
- :CALibration[1]:ZERO:AUTO……56
- :CALibration[1]:ZERO:TYPE……56

:CALibration[1][:ALL]

Function: Zeroing and calibration of the 87235. 1 indicates Channel A and can be omitted.
In which cases is zeroing and calibration required?
Temperature change exceeds 5℃
After the connection is established with the device under test
Restart
Measure small power
every 24 hours. For example, measuring a power 20 dB higher than the minimum power of the 87235.

Query: Not supported

Setting: :CALibration[1][:ALL]

Example: CAL Zeroing and calibration

Error message: If there is an error in zeroing, it prompts "-231, "Data questionable;cal error"".
If there is an error in calibration, it prompts "-231, "Data questionable;zero error"".

:CALibration[1]:AUTO

Function: Calibration of the 87235.

Query: :CALibration[1]:AUTO?

Setting: :CALibration[1]:AUTO <Boolean data>|ONCE|2
Valid forms of <Boolean data> are: 0, OFF, 1, ON.
For ON or 1, parameter retention, the 87235 is NOT supported.
For 0FF or 0, auto-calibration is disabled
For ONCE or 2: Initiate a calibration.

Example: CAL1:AUTO ONCE Calibration of the 87235

Error If there is an error in calibration, it prompts "-231, "Data questionable; cal

message: error"";

Reset state: None

:CALibration[1]:ZERO:AUTO

Function: Zeroing of the 87235. 1 indicates Channel A and can be omitted.

Query: :CALibration[1]:ZERO:AUTO?

Setting: :CALibration[1]:ZERO:AUTO <Boolean data>|ONCE|2

Valid forms of <Boolean data> are: 0, OFF, 1, ON.

For ON or 1, the 87235 enables auto-zero for instant zero drift measurements in real time. Real-time zero drift measurement is only valid for normal measurement mode.

For 0FF or 0, auto-zero is disabled.

For ONCE or 2: Initiate a zeroing.

Example: CAL:ZERO:AUTO ONCE Zero Channel A of the 87235

Error message: If there is an error in zeroing, it prompts "-231, "Data questionable;zero error"".

Reset state: None

:CALibration[1]:ZERO:TYPE

Function: Query or set the zeroing type.

Query: :CALibration[1]:ZERO:TYPE?

Setting: :CALibration[1]:ZERO:TYPE <character data>

Character data is defined as follows:

INTernal or 0: Internal zeroing

EXTernal or 1: External zeroing

Example: CAL:ZERO:TYPE? Query the zeroing type of the 87235

CAL:ZERO:TYPE EXT Set the zeroing of the 87235 to "external"

Error message: None

Reset state: Internal zeroing.

3.3.3 Measurement Subsystem Command (CONFigure/FETCh/READ/MEASure)

Generally, unless otherwise specified, the linear power is in W, the logarithmic power is in dBm, the linear power ratio is in %, the logarithmic power ratio is in dB, and the time is in s.

If the returned value is invalid, NAN (9.91E37) is returned, as defined in IEEE 754.

The differences between the FETCh command, MEASure command, and READ command are as follows:

The FETCh command is to query the displayed value of a given measurement. The execution speed of the FETCh command is not related to the power level and generally

returns immediately. The FETCh command may return intermediate results in the power measurement process rather than the actual power value.

The MEASure command starts a measurement and returns the result only after the measurement is completed. Generally, the lower the power, the longer the MEASure command takes.

The READ command completes a new measurement in the stop state, and INIT:CONT must be set to OFF.

Note: If the trigger source is INT or EXT, after entering a new INIT operation, if the trigger conditions are not met and the trigger signal has not been waited for, the effect is that the device will be hung and the programmed command will not respond. Therefore, when using the measurement subsystem command, it is important to ensure that the device captures the trigger signal.

Commands include:

- :FETCh[1]|2|3|4[:SCALar][:POWer][:AC]?.....57
- :FETCh[1]|2|3|4[:SCALar][:POWer][:AC]:DIFFerence?.....58
- :FETCh[1]|2|3|4[:SCALar][:POWer][:AC]:DIFFerence:RELative?.....58
- :FETCh[1]|2|3|4[:SCALar][:POWer][:AC]:RATio?.....59
- :FETCh[1]|2|3|4[:SCALar][:POWer][:AC]:RATio:RELative?.....59
- :FETCh[1]|2|3|4[:SCALar][:POWer][:AC]:RELative?.....60
- :MEASure[1]|2|3|4[:SCALar][:POWer][:AC]?.....60
- :MEASure[1]|2|3|4[:SCALar][:POWer][:AC]:DIFFerence?.....61
- :MEASure[1]|2|3|4[:SCALar][:POWer][:AC]:DIFFerence:RELative?.....61
- :MEASure[1]|2|3|4[:SCALar][:POWer][:AC]:RATio?.....62
- :MEASure[1]|2|3|4[:SCALar][:POWer][:AC]:RATio:RELative?.....62
- :MEASure[1]|2|3|4[:SCALar][:POWer][:AC]:RELative? 63
- :READ[1]|2|3|4[:SCALar][:POWer][:AC]?.....63
- :READ[1]|2|3|4[:SCALar][:POWer][:AC]:DIFFerence?.....63
- :READ[1]|2|3|4[:SCALar][:POWer][:AC]:DIFFerence:RELative?.....64
- :READ[1]|2|3|4[:SCALar][:POWer][:AC]:RATio?.....64
- :READ[1]|2|3|4[:SCALar][:POWer][:AC]:RATio:RELative?.....65
- :READ[1]|2|3|4[:SCALar][:POWer][:AC]:RELative?.....65

:FETCh[1]|2|3|4[:SCALar][:POWer][:AC]?

Function: Set the specified measurement as absolute power measurement, turn off relative measurement, and return to the measurement value displayed in the current measurement. The measurement unit is specified by UNIT[1]|2|3|4:POWer. This command does not wait for a measurement to be completed before returning. To get the exact measurement value, use the MEAS command.

Query: :FETCh[1]|2|3|4[:SCALar][:POWer][:AC]? [<expected value>[, <resolution>[,

<source channel list>]]]

Set to absolute power measurement, and turn off relative measurement. where both the expected value and the resolution can be expressed as DEF, indicating no change. The resolution ranges from 1 to 4; the channel list is of the form: (@1), indicating Channel A.

Setting: Not supported

Example: FETC2? Query that Measurement 2 is the absolute power measurement value.

Error message: If the last measurement is invalid, it prompts -230, "Data corrupt or stale". Running the INIT command will ensure that the measurement is valid, and changes in measurement parameters (e.g., frequency, channel offset) will cause the measurement to be invalid.

:FETCh[1]|2|3|4[:SCALar][:POWer][:AC]:DIFFerence?

Function: Set the specified measurement as differential power measurement, turn off relative measurement, and return the measured value. The measurement unit is specified by UNIT[1]|2|3|4:POWer. This command does not wait for a measurement to be completed before returning. To get the exact measurement value, use the MEAS command.

Query: :FETCh[1]|2|3|4[:SCALar][:POWer][:AC]:DIFFerence? [<expected value>[, <resolution>[, <source channel list>]]]

Set to differential power measurement and turn off relative measurement. where both the expected value and the resolution can be expressed as DEF, indicating no change. The resolution ranges from 1 to 4; the source channel list is of the form

(@1), (@1), indicating Channel A - Channel A.

Setting: Not supported

Example: FETC3:DIFF? DEF, 3, (@1), (@1) Set Measurement 3 to differential power measurement (Channel A - channel

A) with a resolution of 3, turn off relative measurement, and return the power measurement value.

Error message: If the last measurement is invalid, it prompts -230, "Data corrupt or stale". Running the INIT command will ensure that the measurement is valid, and changes in measurement parameters (e.g., frequency, channel offset) will cause the measurement to be invalid.

:FETCh[1]|2|3|4[:SCALar][:POWer][:AC]:DIFFerence:RELative?

Function: Set the specified measurement as differential power measurement, turn on relative measurement, and return the measured value. The measurement unit is specified by UNIT[1]|2|3|4:POWer:RATio. This command does not wait for a measurement to be completed before returning. To get the exact measurement value, use the MEAS command.

Query: :FETCh[1]|2|3|4[:SCALar][:POWer][:AC]:DIFFerence:RELative? [<expected value>[, <resolution>[, <source channel list>]]]

Set to differential power measurement, and turn on relative measurement. where both the expected value and the resolution can be expressed as DEF, indicating no change. The resolution ranges from 1 to 4; the source channel list is of the form

(@1), (@1), indicating Channel A - Channel A.

Setting: Not supported

Example: FETC3:DIFF:REL? DEF,3,(@1),(@1) Set Measurement 3 to differential power measurement (Channel A - Channel A) with a resolution of 3, turn on relative measurement, and return the power measurement value.

Error message: If the last measurement is invalid, it prompts -230, "Data corrupt or stale". Running the INIT command will ensure that the measurement is valid, and changes in measurement parameters (e.g., frequency, channel offset) will cause the measurement to be invalid.

:FETCh[1]|2|3|4[:SCALar][:POWer][:AC]:RATio?

Function: Set the power measurement mode of the specified measurement as ratio measurement, turn off relative measurement, and return the measured value. The measurement unit is specified by UNIT[1]|2|3|4:POWer:RATio. This command does not wait for a measurement to be completed before returning. To get the exact measurement value, use the MEAS command.

Query: :FETCh[1]|2|3|4[:SCALar][:POWer][:AC]:RATio? [<expected value>[, <resolution>[, <source channel list>]]]

Set to ratio power measurement, where both the expected value and the resolution can be expressed as DEF, indicating no change. The resolution ranges from 1 to 4; the channel list is of the form:

(@1), (@1), indicating Channel A divided by Channel A.

Setting: Not supported

Example: FETC4:RAT? DEF, 3, (@1), (@1) Set measurement 4 to ratio power measurement (Channel A divided by Channel A), and turn off relative measurement, with a resolution of 3. Return the measured value.

Error message: If the last measurement is invalid, it prompts -230, "Data corrupt or stale". Running the INIT command will ensure that the measurement is valid, and changes in measurement parameters (e.g., frequency, channel offset) will cause the measurement to be invalid.

:FETCh[1]|2|3|4[:SCALar][:POWer][:AC]:RATio:RELative?

Function: Set the power measurement mode of the specified measurement as ratio measurement, turn on relative measurement, and return the measured value. The measurement unit is specified by UNIT[1]|2|3|4:POWer:RATio. This command does not wait for a measurement to be completed before returning. To get the exact measurement value, use the MEAS command.

Query: :FETCh[1]|2|3|4[:SCALar][:POWer][:AC]:RATio:RELative? [<expected value>[, <resolution>[, <source channel list>]]]

Set to ratio power measurement, where both the expected value and the resolution can be expressed as DEF, indicating no change. The resolution ranges from 1 to 4; the channel list is of the form:

(@1), (@1), indicating Channel A divided by Channel A.

Setting: Not supported

Example: FETC4:RAT:REL? DEF, 3, (@1), (@1) — Set measurement 4 to ratio power measurement (Channel A divided by Channel A), and turn on relative measurement, with a resolution of 3. Return the measured value

Error message: If the last measurement is invalid, it prompts -230, "Data corrupt or stale". Running the INIT command will ensure that the measurement is valid, and changes in measurement parameters (e.g., frequency, channel offset) will cause the measurement to be invalid.

:FETCh[1]|2|3|4[:SCALar][:POWer][:AC]:RELative?

Function: Set the specified measurement as absolute power measurement, turn on relative measurement, and return the measured value. The measurement unit is specified by UNIT[1]|2|3|4:POWer:RATio. This command does not wait for a measurement to be completed before returning. To get the exact measurement value, use the MEAS command.

Query: :FETCh[1]|2|3|4[:SCALar][:POWer][:AC]:RELative? [<expected value>[, <resolution>[, <source channel list>]]]

Set to absolute power measurement, and turn off relative measurement. where both the expected value and the resolution can be expressed as DEF, indicating no change. The resolution ranges from 1 to 4; the channel list is of the form: (@1), indicating Channel A.

Setting: Not supported

Example: FETC2:REL? — Query the relative power measurement value of Measurement 2.

Error message: If the last measurement is invalid, it prompts -230, "Data corrupt or stale". Running the INIT command will ensure that the measurement is valid, and changes in measurement parameters (e.g., frequency, channel offset) will cause the measurement to be invalid.

:MEASure[1]|2|3|4[:SCALar][:POWer][:AC]?

Function: Set the specified measurement as absolute power measurement, turn off relative measurement, and return the measured value. The measurement unit is specified by UNIT[1]|2|3|4:POWer. Start a measurement and return the measured value when the measurement is completed. And the corresponding FETCh command returns the current measurement value, not when the measurement is completed. When composing a test system, please use the MEASure command.

Query: :MEASure[1]|2|3|4[:SCALar][:POWer][:AC]? [<expected value>[, <resolution>[, <source channel list>]]]

Set to absolute power measurement, and turn off relative measurement. where both the expected value and the resolution can be expressed as DEF, indicating no change. The resolution ranges from 1 to 4; the channel list is of the form: (@1), indicating Channel A.

Setting: Not supported

Example: MEAS2? — Start one measurement and return to Measurement 2 for the absolute power measurement after the measurement is completed.

Error message:

:MEASure[1]|2|3|4[:SCALar][:POWer][:AC]:DIFFerence?

Function: Set the specified measurement as differential power measurement, turn off relative measurement, and return the measured value. The measurement unit is specified by UNIT[1]|2|3|4:POWer. Start a measurement and return the measured value when the measurement is completed. And the corresponding FETCh command returns the current measurement value, not when the measurement is completed. When composing a test system, please use the MEASure command.

Query: :MEASure[1]|2|3|4[:SCALar][:POWer][:AC]:DIFFerence? [<expected value>[, <resolution>[, <source channel list>]]]

Set to differential power measurement and turn off relative measurement. where both the expected value and the resolution can be expressed as DEF, indicating no change. The resolution ranges from 1 to 4; the source channel list is of the form

(@1), (@1), indicating Channel A - Channel A.

Setting: Not supported

Example: MEAS3:DIFF? DEF, 3, (@1), (@1) — Set Measurement 3 to differential power measurement (Channel A - Channel A) with a resolution of 3, turn off relative measurement, start one measurement, and return the power measurement value when the measurement is complete.

Error message:

:MEASure[1]|2|3|4[:SCALar][:POWer][:AC]:DIFFerence:RELative?

Function: Set the specified measurement as differential power measurement, turn on relative measurement, and return the measured value. The measurement unit is specified by UNIT[1]|2|3|4:POWer:RATio. Start a measurement and return the measured value when the measurement is completed. And the corresponding FETCh command returns the current measurement value, not when the measurement is completed. When composing a test system, please use the MEASure command.

Query: :MEASure[1]|2|3|4[:SCALar][:POWer][:AC]:DIFFerence:RELative? [<expected value>[, <resolution>[, <source channel list>]]]

Set to differential power measurement, and turn on relative measurement. where both the expected value and the resolution can be expressed as DEF, indicating no change. The resolution ranges from 1 to 4; the source channel list is of the form

(@1), (@1), indicating Channel A - Channel A.

Setting: Not supported

Example: MEAS3:DIFF:REL? DEF, 3, (@1), (@1) — Set Measurement 3 to differential power measurement (Channel A - Channel A) with a resolution of 3, turn on relative measurement, start one measurement, and return the power measurement value

when the measurement is complete.

Error message:

:MEASure[1]|2|3|4[:SCALar][:POWer][:AC]:RATio?

Function: Set the power measurement mode of the specified measurement as ratio measurement, turn off relative measurement, and return the measured value. The measurement unit is specified by UNIT[1]|2|3|4:POWer:RATio. Start a measurement and return the measured value when the measurement is completed. And the corresponding FETCh command returns the current measurement value, not when the measurement is completed. When composing a test system, please use the MEASure command.

Query: :MEASure[1]|2|3|4[:SCALar][:POWer][:AC]:RATio? [<expected value>[, <resolution>[, <source channel list>]]]

Set to ratio power measurement, where both the expected value and the resolution can be expressed as DEF, indicating no change. The resolution ranges from 1 to 4; the channel list is of the form:

(@1), (@1), indicating Channel A divided by Channel A.

Setting: Not supported

Example: MEAS4:RAT? DEF, 3, (@1), (@1) Set measurement 4 to ratio power measurement (Channel A divided by Channel A), and turn off relative measurement, with a resolution of 3. Start a measurement and return the power measurement value when the measurement is completed.

Error message:

:MEASure[1]|2|3|4[:SCALar][:POWer][:AC]:RATio:RELative?

Function: Set the power measurement mode of the specified measurement as ratio measurement, turn on relative measurement, and return the measured value. The measurement unit is specified by UNIT[1]|2|3|4:POWer:RATio. Start a measurement and return the measured value when the measurement is completed. And the corresponding FETCh command returns the current measurement value, not when the measurement is completed. When composing a test system, please use the MEASure command.

Query: :MEASure[1]|2|3|4[:SCALar][:POWer][:AC]:RATio:RELative? [<expected value>[, <resolution>[, <source channel list>]]]

Set to ratio power measurement, where both the expected value and the resolution can be expressed as DEF, indicating no change. The resolution ranges from 1 to 4; the channel list is of the form:

(@1), (@1), indicating Channel A divided by Channel A.

Setting: Not supported

Example: MEAS4:RAT:REL? DEF, 3, (@1), (@1) Set measurement 4 to ratio power measurement (Channel A divided by Channel A), and turn on relative measurement, with a resolution of 3. Start a measurement and return the

power measurement value when the measurement is completed.

Error message:

:MEASure[1]|2|3|4[:SCALar][:POWer][:AC]:RELative?

Function: Set the specified measurement as absolute power measurement, turn on relative measurement, and return the measured value. The measurement unit is specified by UNIT[1]|2|3|4:POWer. Start a measurement and return the measured value when the measurement is completed. And the corresponding FETCh command returns the current measurement value, not when the measurement is completed. When composing a test system, please use the MEASure command.

Query: :MEASure[1]|2|3|4[:SCALar][:POWer][:AC]:RELative? [<expected value>[, <resolution>[, <source channel list>]]]

Set to absolute power measurement, and turn off relative measurement. where both the expected value and the resolution can be expressed as DEF, indicating no change. The resolution ranges from 1 to 4; the channel list is of the form: (@1) indicating Channel A.

Setting: Not supported

Example: MEAS2:REL? Start a measurement and return the relative power measurement of Measurement 2 when the measurement is completed.

Error message:

:READ[1]|2|3|4[:SCALar][:POWer][:AC]?

Function: Set the specified measurement as absolute power measurement, turn off relative measurement, and return the measured value. The measurement unit is specified by UNIT[1]|2|3|4:POWer.

Query: :READ[1]|2|3|4[:SCALar][:POWer][:AC]? [<expected value>[, <resolution>[, <source channel list>]]]

Set to absolute power measurement, and turn off relative measurement. where both the expected value and the resolution can be expressed as DEF, indicating no change. The resolution ranges from 1 to 4; the channel list is of the form: (@1), indicating Channel A.

Setting: Not supported

Example: READ2? Query that Measurement 2 is the absolute power measurement value.

Error message: If INIT:CONT is set to ON, it prompts -213, "Init ignored".

:READ[1]|2|3|4[:SCALar][:POWer][:AC]:DIFFerence?

Function: Set the specified measurement as differential power measurement, turn off relative measurement, and return the measured value. The measurement unit is specified by UNIT[1]|2|3|4:POWer.

Query: :READ[1]|2|3|4[:SCALar][:POWer][:AC]:DIFFerence? [<expected value>[,

<resolution>[, <source channel list>]]]

Set to differential power measurement and turn off relative measurement. where both the expected value and the resolution can be expressed as DEF, indicating no change. The resolution ranges from 1 to 4; the source channel list is of the form

(@1), (@1), indicating Channel A - Channel A.

Setting: Not supported

Example: READ3:DIFF? DEF, 3, (@1), (@1) Set Measurement 3 to differential power measurement (Channel A - Channel A) with a resolution of 3, turn off relative measurement, and return the power measurement value.

Error message: If INIT:CONT is set to ON, it prompts -213, "Init ignored".

:READ[1]|2|3|4[:SCALar][:POWer][:AC]:DIFFerence:RELative?

Function: Set the specified measurement as differential power measurement, turn on relative measurement, and return the measured value. The measurement unit is specified by UNIT[1]|2|3|4:POWer:RATio.

Query: :READ[1]|2|3|4[:SCALar][:POWer][:AC]:DIFFerence:RELative? [<expected value>[, <resolution>[, <source channel list>]]]

Set to differential power measurement, and turn on relative measurement. where both the expected value and the resolution can be expressed as DEF, indicating no change. The resolution ranges from 1 to 4; the source channel list is of the form

(@1), (@1), indicating Channel A - Channel A.

Setting: Not supported

Example: READ3:DIFF:REL? DEF, 3, (@1), (@1) Set Measurement 3 to differential power measurement (Channel A - Channel A) with a resolution of 3, turn on relative measurement, and return the power measurement value.

Error message: If INIT:CONT is set to ON, it prompts -213, "Init ignored".

:READ[1]|2|3|4[:SCALar][:POWer][:AC]:RATio?

Function: Set the power measurement mode of the specified measurement as ratio measurement, turn off relative measurement, and return the measured value. The measurement unit is specified by UNIT[1]|2|3|4:POWer:RATio.

Query: :READ[1]|2|3|4[:SCALar][:POWer][:AC]:RATio [<expected value>[, <resolution>[, <source channel list>]]]

Set to ratio power measurement, where both the expected value and the resolution can be expressed as DEF, indicating no change. The resolution ranges from 1 to 4; the channel list is of the form:

(@1), (@1), indicating Channel A divided by Channel A.

Setting: Not supported

Example: READ4:RAT? DEF, 3, (@1), Set measurement 4 to ratio power measurement (Channel A divided by

	(@1)	Channel A), and turn off relative measurement, with a resolution of 3. Return the measured value.

Error message: If INIT:CONT is set to ON, it prompts -213, "Init ignored".

:READ[1]|2|3|4[:SCALar][:POWer][:AC]:RATio:RELative?

Function: Set the power measurement mode of the specified measurement as ratio measurement, turn on relative measurement, and return the measured value. The measurement unit is specified by UNIT[1]|2|3|4:POWer:RATio.

Query: :READ[1]|2|3|4[:SCALar][:POWer][:AC]:RATio:RELative? [<expected value>[, <resolution>[, <source channel list>]]]

Set to ratio power measurement, where both the expected value and the resolution can be expressed as DEF, indicating no change. The resolution ranges from 1 to 4; the channel list is of the form:

(@1), (@1), indicating Channel A divided by Channel A.

Setting: Not supported

Example:	READ4:RAT:REL? DEF, 3, (@1), (@1)	Set measurement 4 to ratio power measurement (Channel A divided by Channel A), and turn on relative measurement, with a resolution of 3. Return the measured value.

Error message: If INIT:CONT is set to ON, it prompts -213, "Init ignored".

:READ[1]|2|3|4[:SCALar][:POWer][:AC]:RELative?

Function: Set the specified measurement as absolute power measurement, turn on relative measurement, and return the measured value. The measurement unit is specified by UNIT[1]|2|3|4:POWer:RATio.

Query: :READ[1]|2|3|4[:SCALar][:POWer][:AC]:RELative? [<expected value>[, <resolution>[, <source channel list>]]]

Set to absolute power measurement, and turn off relative measurement. where both the expected value and the resolution can be expressed as DEF, indicating no change. The resolution ranges from 1 to 4; the channel list is of the form: (@1) indicating Channel A.

Setting: Not supported

Example:	READ2:REL?	Query the relative power measurement value of Measurement 2.

Error message: If INIT:CONT is set to ON, it prompts -213, "Init ignored".

3.3.4 Display Subsystem Command (DISPlay)

The DISPlay subsystem is used to control the display of text, graphics and traces.

Commands include:

:DISPlay[:WINDow[1]|2][:NUMeric[1]|2]:RESolution

Function: Query or set the display resolution of the specified measurement. WINDow1

indicates the upper window, which can be omitted, and WINDow2 indicates the lower window; NUMeric1 indicates the upper measurement, which can be omitted, and NUMeric2 indicates the lower measurement.

Query: :DISPlay[:WINDow[1]|2][:NUMeric[1]|2]:RESolution? [MIN|MAX]

Setting: :DISPlay[:WINDow[1]|2][:NUMeric[1]|2]:RESolution <numeric data>
Valid values for numeric data are: DEF, MIN, MAX, <NRf>, where DEF and <NRf> are used for setting only.
<NRf> ranges from 1 to 4.

Example:

DISP:WIND2:NUM2:RES?	Query the display resolution of Measurement 4.
DISP:RES 3	Set the display resolution of Measurement 1 to 3, i.e., display 3 valid digits for linear display and 2 decimal places (0.01) for logarithmic display.

Reset state: Resolution is 3

3.3.5 Format Subsystem Command (FORMat)

The format subsystem is used to set the transmission format of the numeric data. This format system is only used for the following query commands:

FETCh?

MEASure?

READ?

- :FORMat[:READings]:BORDer.....66
- :FORMat[:READings][:DATA].....66

:FORMat[:READings]:BORDer

Function: Query or set the transmission order of binary data: normal or byte exchange.
Valid only when FORMat[:READings][:DATA] is set to REAL.

Query: :FORMat[:READings]:BORDer?

Setting: :FORMat[:READings]:BORDer <character data>
Valid values for <character data> are: 0 or NORMal, 1 or SWAPped

Example:

FORM:BORD?	Query the transmission order.
FORM:BORD SWAP	Set the transmission order to byte-swap.

Reset state: Set to NORMal

:FORMat[:READings][:DATA]

Function: Query or set the data transfer format: ASCii and REAL (real numbers)

Query: :FORMat[:READings][:DATA]?

Setting: :FORMat[:READings][:DATA] <character data>
Valid values for <character data> are: 0 or ASCii, 1 or REAL
ASCii: Numerical data is transferred in the form of <NRf>.

REAL: Numerical data is transferred in IEEE 754 64-bit floating point format and is 8 bytes per data.

Example: FORM? Query the data transmission format.

FORM REAL Set the data transmission format to REAL.

Reset state: Set to ASCii

3.3.6 Memory Subsystem Command (MEMory/MMEMory)

- :MEMory:CATalog[:ALL]?....67
- :MEMory:CATalog:STATe?....68
- :MEMory:CATalog:TABLe?....68
- :MEMory:CLEar[:NAME]....68
- :MEMory:CLEar:TABLe[1]|2|3|4|5|6|7|8|9|10....69
- :MEMory:FREE[:ALL]?....69
- :MEMory:FREE:STATe?....69
- :MEMory:FREE:TABLe?....70
- :MEMory:NSTates?....70
- :MEMory:STATe:CATalog?....70
- :MEMory:STATe:DEFine....70
- :MEMory:TABLe[1]|2|3|4|5|6|7|8|9|10:DEFine....70
- :MEMory:TABLe[1]|2|3|4|5|6|7|8|9|10:FREQuency....71
- :MEMory:TABLe[1]|2|3|4|5|6|7|8|9|10:FREQuency:POINts?....71
- :MEMory:TABLe[1]|2|3|4|5|6|7|8|9|10:GAIN[:MAGNitude]....71
- :MEMory:TABLe[1]|2|3|4|5|6|7|8|9|10:GAIN[:MAGNitude]:POINts?....72
- :MEMory:TABLe:MOVE....72
- :MEMory:TABLe:SELect....72

:MEMory:CATalog[:ALL]?

Function: Enumerate the user configurations in the 87235, including storage call configuration, frequency response offset table (FDO), etc.

The data format is: <value 1>, <value 2> {, <string>}

Where <value 1> indicates the length of bytes used by the user configuration and <value 2> indicates the length of unused bytes.

The form of each <string> is as follows:

<string i>, <type>, <length>

<string i> indicates the name of the user configuration.

<type> indicates the type of user configuration, TABL indicates frequency response offset table, and STAT indicates store call configuration.

<length> indicates the length in bytes of this configuration item.

Query: :MEMory:CATalog[:ALL]?

Setting: Not supported

Example: MEM:CAT? Enumerate all user configurations in the 87235.

Reset state: None

:MEMory:CATalog:STATe?

Function: Enumerate the storage call configuration in the 87235.

The data format is: <value 1>, <value 2> {, <string>}

Where <value 1> indicates the length of bytes used by the user configuration and <value 2> indicates the length of unused bytes.

The form of each <string> is as follows:

<string i>, <type>, <length>

<string i> indicates the name of the user configuration.

<type> indicates the type of user configuration, and STAT indicates store call configuration.

<length> indicates the length in bytes of this configuration item.

Query: :MEMory:CATalog:STATe?

Setting: Not supported

Example: MEM:CAT:STAT? Enumerate the storage call configuration in the 87235.

:MEMory:CATalog:TABLe?

Function: Enumerate the frequency response offset table in the 87235.

The data format is: <value 1>, <value 2> {, <string>}

Where <value 1> indicates the length of bytes used by the user configuration and <value 2> indicates the length of unused bytes.

The form of each <string> is as follows:

<string i>, <type>, <length>

<string i> indicates the name of the user configuration.

<type> indicates the type of user configuration, and TABL indicates frequency response offset table.

<length> indicates the length in bytes of this configuration item.

Query: :MEMory:CATalog:TABLe?

Setting: Not supported

Example: MEM:CAT:TABL? Enumerate the frequency response offset table in the 87235.

:MEMory:CLEar[:NAME]

Function: Used to clear the frequency response offset table or storage call table specified in the power.

Query: Not supported

Setting: :MEMory:CLEar[:NAME] <string>

<string> indicates the name of frequency response offset table or storage

call table

Example: MEM:CLE "fdo0" Clear the fdo0 frequency response offset table.

Description: 1) If the specified frequency response offset table is enabled, it is automatically turned off.

2) The English name of the storage call state is "State1", "State2" ..... "State10", and the name cannot be changed. The Chinese name of the storage call state is "State 1", "State 2" ..... "State 10", and the name cannot be changed.

3) Clear the frequency response offset table if the specified name can be found in the frequency response bias list;

4) Clear the state table if the specified name can be found in the storage call state list.

5) If there is a frequency response bias of "State1", then call MEM:CLE "State1", which will clear the frequency response offset table and state table.

6) In the program control setting, the state name of the storage call has no relationship with the language switch of the interface, i.e., the following two commands both clear the state 1 (English name is recommended).

MEM:CLE "State 1"

MEM:CLE "State1"

Error message: If the specified name does not exist, it prompts "-224, "Illegal parameter value""

Reset state: None

:MEMory:CLEar:TABLe[1]|2|3|4|5|6|7|8|9|10

Function: Clear the specified frequency response offset table.

Query: Not supported

Setting: :MEMory:CLEar:TABLe[1]|2|3|4|5|6|7|8|9|10

Example: MEM:CLE:TABL5 Clear the 5th frequency response offset table. (10 in total)

:MEMory:FREE[:ALL]?

Function: Query the total number of bytes unused in the user configuration space and the number of bytes used.

The return string is of the form: <unused bytes>, <used bytes>

Query: :MEMory:FREE[:ALL]?

Setting: Not supported

Example: MEM:FREE?

:MEMory:FREE:STATe?

Function: Query the total number of bytes unused in the storage call space and the number of bytes used.

The return string is of the form: <unused bytes>, <used bytes>

Query: :MEMory:FREE:STATe?

Setting: Not supported

Example: MEM:FREE:STAT?

:MEMory:FREE:TABLe?

Function: Query the total number of unused bytes and the number of bytes used in the frequency response offset table space.

The return string is of the form: <unused bytes>, <used bytes>

Query: :MEMory:FREE:TABLe?

Setting: Not supported

Example: MEM:FREE:TABL?

:MEMory:NSTates?

Function: Query the number of storage call states, and always return 10

Query: :MEMory:NSTates?

Setting: Not supported

Example: MEM:NST?

:MEMory:STATe:CATalog?

Function: Enumerate the names of all storage call states.

Query: :MEMory:STATe:CATalog?

Setting: Not supported

Example: MEM:STAT:CAT?

:MEMory:STATe:DEFine

Function: Query or set the name of the storage call status register.

Query: :MEMory:STATe:DEFine? <string>

The string is the name of the instrument status contained in matching quotation marks.

Setting: :MEMory:STATe:DEFine <string>, <numeric data>

The definition of string is the same as that of query format;

Valid values for numeric data are: DEF, MIN, MAX, <NRf>, where DEF and <NRf> are used for setting only.

<NRf> ranges from 1 to 10.

Example: MEM:STAT:DEF? "State1" Query the state register number corresponding to the "State1".

MEM:STAT:DEF? "MyState",8 Name the state register 8 as "MyState"

:MEMory:TABLe[1]|2|3|4|5|6|7|8|9|10:DEFine

Function: Query or set the name in the specified frequency response offset table.

Query: :MEMory:TABLe[1]|2|3|4|5|6|7|8|9|10:DEFine?

Setting: :MEMory:TABLe[1]|2|3|4|5|6|7|8|9|10:DEFine <string>

Example:	MEM:TABL6:DEF?	Query the name of the 6th frequency response offset table.
	MEM:TABL8:DEF "fdo0"	Name the 8th frequency response offset table as fdo0.

Error message: If the specified name already exists, it prompts "-257, "File name error"".

:MEMory:TABLe[1]|2|3|4|5|6|7|8|9|10:FREQuency

Function: Query or set the frequency list in the specified frequency response offset table.

When setting the frequency list, the previous frequency list will be cleared and the frequency list must be sorted in ascending order.

The relevant command is:MEMory:TABLe[1]|2|3|4|5|6|7|8|9|10:GAIN[:MAGNitude]

Query: :MEMory:TABLe[1]|2|3|4|5|6|7|8|9|10:FREQuency?

Setting: :MEMory:TABLe[1]|2|3|4|5|6|7|8|9|10:FREQuency <numeric data 1>{, <numeric data n>}

It is necessary to ensure that this frequency list covers the frequency range of the 87235, and if the frequency of the signal under test is outside the range of this list, the value at the lowest or highest frequency will be used.

The maximum number of frequency points is 80.

The effective units of frequency are: Hz, kHz, MHz, and GHz

Example:	MEM:TABL6:FREQ?	Query the frequency list of the 6th frequency response offset table.
	MEM:TABL6:FREQ 50MHz, 40GHz	Set the frequency of the 6th frequency response offset table to 50MHz and 40GHz.

Error message: If the number of points in the frequency list exceeds 80, it prompts "-108, "Parameter not allowed"".

If the frequency list is not in increasing order, it prompts "-220, "Parameter error"”

Reset state: None

:MEMory:TABLe[1]|2|3|4|5|6|7|8|9|10:FREQuency:POINts?

Function: Query the frequency points of the frequency response offset table.

Query: :MEMory:TABLe[1]|2|3|4|5|6|7|8|9|10:FREQuency:POINts?

Setting: Not supported

Example:	MEM:TABL6:FREQ:POIN?	Query the frequency points of the 6th frequency response offset table.

:MEMory:TABLe[1]|2|3|4|5|6|7|8|9|10:GAIN[:MAGNitude]

Function: Query or set the amplitude gain list in the specified frequency response offset table.

When setting the gain list, the previous gain list will be cleared,

The related command is:MEMory:TABLe[1]|2|3|4|5|6|7|8|9|10:FREQuency

Query: :MEMory:TABLe[1]|2|3|4|5|6|7|8|9|10:GAIN[:MAGNitude]?

Setting: :MEMory:TABLe[1]|2|3|4|5|6|7|8|9|10:GAIN[:MAGNitude] <numeric data >{, <numeric data >}

The maximum gain points is 80.

It is in PCT, i.e. 100 means 100%

The amplitude gain ranges from 1.0e-009 to 1.0e+009, or -90dB to 90dB.

Example:		
	MEM:TABL6:GAIN?	Query the gain list of the 6th frequency response offset table.
	MEM:TABL6:GAIN 98, 102	Set the gain list of the 6th frequency response offset table to 98% and 102%.

:MEMory:TABLe[1]|2|3|4|5|6|7|8|9|10:GAIN[:MAGNitude]:POINts?

Function: Query the amplitude gain points of the frequency response offset table.

Query: :MEMory:TABLe[1]|2|3|4|5|6|7|8|9|10:GAIN[:MAGNitude]:POINts?

Setting: Not supported

Example:		
	MEM:TABL6:GAIN:POIN?	Query the amplitude gain points of the 6th frequency response offset table

:MEMory:TABLe:MOVE

Function: Rename the specified frequency response offset table. This command requires prior knowledge of the name of the frequency response offset table to be modified.

Related commands MEMory:TABLe[1]|2|3|4|5|6|7|8|9|10:DEFine

It is recommended to use MEMory:TABLe[1]|2|3|4|5|6|7|8|9|10:DEFine.

Query: Not supported

Setting: :MEMory:TABLe:MOVE < string 1>, < string 2>

<string 1> indicates the name of the frequency response offset table that needs to be modified

<string 2> indicates the name of the modified frequency response offset table

Example: MEM:TABL:MOVE "fdo0", "fdo1"

Error message: If the frequency response offset table specified by the first parameter does not exist, it prompts "-256, "File name not found""

If the frequency response offset table specified by the second parameter already exists, it prompts "-257, "File name error"”

If the length of the second parameter is longer than 16 characters, it prompts "-257, "File name error"”

:MEMory:TABLe:SELect

Function: Query or set the current frequency response offset table. This is different from 2434. Calibration table is supported in 2434, and this command can be used to select a calibration table.

Query: :MEMory:TABLe:SELect?

Setting:	:MEMory:TABLe:SELect <string>	
Example:	MEM:TABL:SEL?	Return the name of the current frequency response offset table.
	MEM:TABL:SEL "fdo0"	Set the current frequency response offset table to fdo0.
Error message:	If the frequency response offset table specified by the parameter does not exist, it prompts "-224, "Illegal parameter value"".	

3.3.7 Sensor Subsystem Command (SENSe)

- [:SENSe[1]:]AVERage[1]|2:COUNt....74
- [:SENSe[1]:]AVERage:COUNt:AUTO....75
- [:SENSe[1]:]AVERage:RESet....75
- [:SENSe[1]:]AVERage:SDETect....75
- [:SENSe[1]:]AVERage[1]|2[:STATe]....75
- [:SENSe[1]:]BANDwidth|BWIDth:VIDeo....76
- [:SENSe[1]:]BUFFer:COUNt....76
- [:SENSe[1]:]BUFFer:MTYPe....77
- [:SENSe[1]:]CORRection:CSET2[:SELect]....77
- [:SENSe[1]:]CORRection:CSET2:STATe....78
- [:SENSe[1]:]CORRection:DCYCle[:INPut][:MAGNitude]....78
- [:SENSe[1]:]CORRection:FDOFfset[:INPut][:MAGNitude]?....78
- [:SENSe[1]:]CORRection:DCYCle[:INPut]:STATe....78
- [:SENSe[1]:]CORRection:GAIN[1]|2|3|4[:INPut][:MAGNitude]....79
- [:SENSe[1]:]CORRection:GAIN[1]|2|3|4[:INPut]:STATe....80
- [:SENSe[1]:]DETector:FUNCtion....80
- [:SENSe[1]:]FREQuency[:CW|FIXed]....80
- [:SENSe[1]:]FREQuency[:CW|FIXed]:STARt....81
- [:SENSe[1]:]FREQuency[:CW|FIXed]:STEP....81
- [:SENSe[1]:]FREQuency[:CW|FIXed]:STOP....82
- [:SENSe[1]:]LIST:FREQuency:STARt....83
- [:SENSe[1]:]LIST:FREQuency:STOP....83
- [:SENSe[1]:]LIST:MTYPe....84
- [:SENSe[1]:]LIST:POINts....84
- [:SENSe[1]:]LIST:STATe....85
- [:SENSe[1]:]LIST:TSCount....85
- [:SENSe[1]:]LIST:TSLot:EXCLude:OFFSet:TIME....86

- [:SENSe[1]:]LIST:TSLot:EXCLude:TIME....87
- [:SENSe[1]:]LIST:TSLot:TIME....88
- [:SENSe[1]:]LIST:TSLot:TREF[1]|2....88
- [:SENSe[1]:]MRATe....89
- [:SENSe[1]:]POWer:AC:RANGe....89
- [:SENSe[1]:]POWer:AC:RANGe:AUTO....90
- [:SENSe[1]:]SWEep:APERture....90
- [:SENSe[1]:]SWEep:APERture:AUTO....91

[:SENSe[1]:]AVERage[1]|2:COUNt

Function: Query or set the average number of measurements and the average number of videos.

AVERage [1]: measurement average, where consecutive measurements are averaged in order to improve the accuracy of the measurements.

Setting this command will automatically perform the following command settings:

AVERage:COUNt:AUTO OFF

AVERage1:STATe ON

AVERage2: Video average, or trace average, where consecutive traces are averaged without affecting the dynamic range of the signal to reduce the effects of noise.

Setting this command will automatically perform the following command settings:

AVERage2:STATe ON

Query: [:SENSe[1]:]AVERage[1]|2:COUNt? [MIN|MAX]

Setting: [:SENSe[1]:]AVERage[1]|2:COUNt <numeric data>

Valid values for numeric data are: DEF, MIN, MAX, <NRf>, where DEF and <NRf> are used for setting only.

<NRf> ranges from 1 to 1024.

DEF is 8,

MIN is 1,

MAX 为 1024.

Example:

SENS1:AVER:COUN?	Query the average number of measurements.
SENS1:AVER2:COUN?	Query the average number of videos.
SENS1:AVER:COUN? MAX	Query the maximum value of the settable average number of measurements.
SENS:AVER:COUN 28	Set the average number of measurements to 28.

Reset state: Average times set to 8.

[:SENSe[1]:]AVERage:COUNt:AUTO

Function: Query or set the measurement auto-average state.

Query: [:SENSe[1]:]AVERage:COUNt:AUTO?

Setting: [:SENSe[1]:]AVERage:COUNt:AUTO <Boolean data>
Valid forms of <Boolean data> are: 0, OFF, 1, ON

Example:

SENS1:AVER:COUN:AUTO?	Query the automatic average status.
SENS:AVER:COUN:AUTO 1	Turn on Auto Average.

Limit:

Error message:

Reset state: Auto Average is set to ON.

[:SENSe[1]:]AVERage:RESet

Function: Clear the averaging buffer and restart averaging of the 87235.
The 87235 is equipped with an internal averaging buffer for storing historical measurement data. This command is used to clear this buffer and re-store it.

Query: Not supported

Setting: [:SENSe[1]:]AVERage:RESet

Example:

AVER:RES	Re-average

Limit:

Reset state:

[:SENSe[1]:]AVERage:SDETect

Function: Query or set the channel step detection state.
In Auto Average mode, the last four averages are used to compare with the entire filter value, and the digital filter is cleared when the difference between the two averages exceeds 15%. The filter then starts storing the new measured values. The use of this function is able to shorten the filtering time when the power changes more significantly.

Query: [:SENSe[1]:]AVERage:SDETect?

Setting: [:SENSe[1]:]AVERage:SDETect <Boolean data>
Valid forms of <Boolean data> are: 0, OFF, 1, ON

Example:

SENS1:AVER:SDET?	Query the step detection state.
SENS:AVER:SDET 1	Turn on the step detection.

Limit:

Reset state: Step detection is set to ON.

[:SENSe[1]:]AVERage[1]|2[:STATe]

Function: Query or set the measurement average and video average switch state.

Query: [:SENSe[1]:]AVERage[1]|2[:STATe]?

Setting: [:SENSe[1]:]AVERage[1]|2[:STATe] <Boolean data>
Valid forms of <Boolean data> are: 0, OFF, 1, ON

Example: SENS1:AVER? Query the measurement average switch status.

SENS:AVER 1 Turn on the measurement average switch.

Reset state: Average state is set to ON.

[:SENSe[1]:]BANDwidth|BWIDth:VIDeo

Function: Query or set the measured video bandwidth.

Query: [:SENSe[1]:]BANDwidth|BWIDth:VIDeo?

Setting: [:SENSe[1]:]BANDwidth|BWIDth:VIDeo <character data>
The valid form of <character data> is as follows:
OFF|0: OFF (>5M)
LOW|1: Low (300kHz)
MEDium|2: Medium (1.5M)
HIGH|3: High (5M)

Example: SENS1:BAND:VID? QueryVBW

BWID:VID 1 VBW is low

BAND:VID HIGH VBW is high

Reset state: VBW is OFF

[:SENSe[1]:]BUFFer:COUNt

Function: Query or set the buffer size of external trigger measurement, which is only used for external trigger measurement.
Note: This command can only be set when
[:SENSe[1]:]FREQuency[:CW|FIXed]:STEP
is set to 0, otherwise an error will be reported.

Query: [:SENSe[1]:]BUFFer:COUNt?

Setting: [:SENSe[1]:]BUFFer:COUNt <numeric data>
Valid values for numeric data are: DEF, MIN, MAX, <NRf>, where DEF and <NRf> are used for setting only.
<NRf> ranges from 1 to 80000
DEF 为 1.
MIN 为 1
MAX 为 80000.

Example: SENS:BUFF:COUN? Query the current buffer size of external trigger measurement.

SENS:BUFF:COUN 100 Set the buffer size of external trigger measurement to 100.

Error If the trigger source (TRIG:SOUR) is not "external trigger", it prompts "-221,

message: "Settings conflict"".

If the number of frequency steps (FREQ:STEP) is not 0, it prompts "-221, "Settings conflict"".

Reset state: 1

[:SENSe[1]:]BUFFer:MTYPe

Function: Query or set the external trigger buffer measurement type, which is only used for external trigger measurement.

Query: [:SENSe[1]:]BUFFer:MTYPe?

Setting: [:SENSe[1]:]BUFFer:MTYPe <string>

<string> can be the following values:

"AVER": average power measurement mode

"PEAK": peak power measurement mode

"PTAV": peak-to-average ratio measurement mode

"MIN": minimum power measurement mode

Example:

BUFF:MTYP?	Query the current buffer measurement type.
SENS:BUFF:MTYP "PEAK"	Set the buffer measurement mode to "Peak".

Error message: If the trigger source (TRIG:SOUR) is not "external trigger", it prompts "-221, "Settings conflict"".

If the parameter is an invalid string, it prompts "-224, "Illegal parameter value"".

If the detection measurement method (SENS:DET:FUNC) is "AVER", the message "-221, it prompts "Settings conflict"".

Reset state: Average power measurement mode

[:SENSe[1]:]CORRection:CSET2[:SELect]

Function: Set or query the name of the frequency response offset table used for the current device.

The data of the frequency response offset table is shared between the two channels, but the switch states are separate.

Query: [:SENSe[1]:]CORRection:CSET2[:SELect]?

Setting: [:SENSe[1]:]CORRection:CSET2[:SELect] <string>

<string> indicates the name of the frequency response offset table.

Example:

SENS:CORR:CSET2?	Query the currently selected frequency response offset table.
SENS:CORR:CSET2 "fdo0"	Select the frequency response offset table named "fdo0".

Error message: If the frequency response offset table specified by the parameter does not exist, it prompts "-256, "File name not found"".

Reset state: No effect.

3.3 Instrument Subsystem Command

[:SENSe[1]:]CORRection:CSET2:STATe

Function: Query or set the enable state of the frequency response offset table.

The data of the frequency response offset table is shared between the two channels, but the enable states are separate.

Query: [:SENSe[1]:]CORRection:CSET2:STATe?

Setting: [:SENSe[1]:]CORRection:CSET2:STATe <Boolean data>

Valid forms of <Boolean data> are: 0, OFF, 1, ON

Example:

SENS1:CORR:CSET2:STAT?	Query the enable state of the frequency response offset table.
SENS:CORR:CSET2:STAT 0	Disable the frequency response offset table.

Error message: If the number of frequency points and the number of amplitude gain (offset) points in the currently selected frequency response offset table are different, it prompts "-226," list length is not the same ""

If the point in the currently selected frequency response offset table is 0, it prompts "-221, "Settings conflict"".

Reset state: Does not affect the to enable state of the frequency response offset table.

[:SENSe[1]:]CORRection:DCYCle[:INPut][:MAGNitude]

Function: Query or set the channel duty cycle setting value for pulse power measurement.

Pulse power measurements average any aberrations such as overshoot, ringing, etc. The measurement is a mathematical representation of the pulse power measurement and not a true measurement. The 87235 measures the average power of the pulse signal by dividing it by the duty cycle to obtain a pulse power reading.

Note: To ensure the accuracy of the measurement, the input signal must be a rectangular pulse, other pulses (such as triangle wave, linear FM pulse) will lead to inaccurate measurement.

The switching ratio of the pulse under test must be much larger than the duty cycle setting.

Query: [:SENSe[1]:]CORRection:DCYCle[:INPut][:MAGNitude]? [MIN|MAX]

Setting: [:SENSe[1]:]CORRection:DCYCle[:INPut][:MAGNitude] <numeric data>

Valid values for numeric data are: DEF, MIN, MAX, <NRf>, where DEF and <NRf> are used for setting only.

<NRf> ranges from 0.001 to 100, in %.

DEF is 100,

MIN is 0.001,

MAX 为 100.

Example:

SENS:CORR:DCYC?	Query the current duty cycle setting value of the channel.
CORR:DCYC? MAX	Query the maximum settable duty cycle.
CORR:DCYC 50	Set the channel duty cycle to 50%.

Reset 100%

state:

[:SENSe[1]:]CORRection:DCYCle[:INPut]:STATe

Function: Query or set the channel duty cycle enable switch for pulse power measurement.

Query: [:SENSe[1]:]CORRection:DCYCle[:INPut]:STATe?

Setting: [:SENSe[1]:]CORRection:DCYCle[:INPut]:STATe <Boolean data>
Valid forms of <Boolean data> are: 0, OFF, 1, ON

Example:

SENS:CORR:DCYC:STAT?	Query the to duty cycle enable state of the channel.
CORR:DCYC:STAT 1	Enable the duty cycle correction for the channel.

Reset state: Off

[:SENSe[1]:]CORRection:FDOFfset[:INPut][:MAGNitude]?

Function: Query the currently used frequency response offset factor. It is in PCT, i.e. 100 means 100%.

Query: [:SENSe[1]:]CORRection:FDOFfset[:INPut][:MAGNitude]?

Setting: Not supported

Example:

CORR:FDOF?	Query the currently used frequency response offset factor.

Limit: Only for USB channel (8), other channels are not supported.

[:SENSe[1]:]CORRection:GAIN[1]|2|3|4[:INPut][:MAGNitude]

Function: Used to set or query four kinds of gains for the current device;
The equivalent form of GAIN [1] is CFACtor, which denotes the calibration factor of the 87235. The former conforms to the SCPI specification, while the latter does not. GAIN [1] is not supported in this case;
GAIN2 indicates the channel offset. It is supported in this case. It can be queried or set.
The equivalent form of GAIN3 is DCYCle, which represents the duty cycle.
The equivalent form of GAIN4 is FDOFfset, which represents the frequency response offset factor. GAIN4 is supported in this case. The frequency response offset factor is only available for query.

Query: [:SENSe[1]:]CORRection:GAIN2|4[:INPut][:MAGNitude]? [MIN|MAX]

Setting: [:SENSe[1]:]CORRection:GAIN2[:INPut][:MAGNitude] <numeric data>
Valid values for numeric data are: DEF, MIN, MAX, <NRf>, where DEF and <NRf> are used for setting only.
<NRf> ranges from -100 to 100, in dB.
DEF is 0dB,
MIN is -100dB,
MAX 为 100dB.

Example:

SENS:CORR:GAIN2?	Query the channel offset.

	CORR:GAIN2? MAX	Query the maximum settable channel offset value.
	SENS1:CORR:GAIN4?	Query the frequency response offset value.
	CORR:GAIN2 3.6	Set the channel offset to 3.6dB.

Reset state: Channel offset is 0; duty cycle is 100%

[:SENSe[1]:]CORRection:GAIN[1]|2|3|4[:INPut]:STATe

Function: The equivalent form of GAIN [1] is CFACtor, which denotes the calibration factor of the 87235. The former conforms to the SCPI specification, while the latter does not. GAIN [1] is not supported in this case;

GAIN2 indicates the channel offset.

The equivalent form of GAIN3 is DCYCle, which represents the duty cycle. GAIN3 is not supported in this case

The equivalent form of GAIN4 is FDOFfset, which represents the frequency response offset factor. This case does not support the query and setting of GAIN4 state.

Query: [:SENSe[1]:]CORRection:GAIN2[:INPut]:STATe?

Setting: [:SENSe[1]:]CORRection:GAIN2[:INPut]:STATe <Boolean data>

Valid forms of <Boolean data> are: 0, OFF, 1, ON

Example:	SENS:CORR:GAIN2:STAT?	Query the channel offset enable state.
	CORR:GAIN2:STAT 1	Enable the channel offset.

Reset state: Off

[:SENSe[1]:]DETector:FUNCtion

Function: Query or set the detection measurement mode of the 87235.

Query: [:SENSe[1]:]DETector:FUNCtion?

Setting: [:SENSe[1]:]DETector:FUNCtion <character data>

The valid values of the character data are as follows:

AVERage or 0: Average power measurement mode

NORMal or 1: Normal peak measurement mode

Example:	DET:FUNC?	Query the measurement method
	DET:FUNC AVER	Set to average power measurement mode.

Reset state: Average power measurement mode.

[:SENSe[1]:]FREQuency[:CW|FIXed]

Function: Query or set the frequency.

Query: [:SENSe[1]:]FREQuency[:CW|FIXed]? [MIN|MAX]

Setting: [:SENSe[1]:]FREQuency[:CW|FIXed] <numeric data>

Valid values for numeric data are: DEF, MIN, MAX, <NRf>, where DEF and

<NRf> are used for setting only.
<NRf> ranges 1e3 to 1e12, in Hz,
DEF is 1GHz,
MIN is 1kHz,
MAX is 1000GHz,

Example:	FREQ?	Query the frequency.
	FREQ? MAX	Query the maximum settable frequency.
	SENS:FREQ 8GHz	Set the frequency to 8GHz.

Reset state: 1GHz.

[:SENSe[1]:]FREQuency[:CW|FIXed]:STARt

Function: Query or set the frequency for the start frequency of the external trigger buffer sweep measurement.

Associated commands:
[:SENSe[1]:]FREQuency[:CW|FIXed]:STOP
[:SENSe[1]:]FREQuency[:CW|FIXed]:STEP
The start frequency can be greater than or equal to the stop frequency.

Query: [:SENSe[1]:]FREQuency[:CW|FIXed]:STARt? [MIN|MAX]

Setting: [:SENSe[1]:]FREQuency[:CW|FIXed]:STARt <numeric data>
Valid values for numeric data are: DEF, MIN, MAX, <NRf>, where DEF and <NRf> are used for setting only.
<NRf> ranges 1e3 to 1e12, in Hz,
DEF is 1GHz,
MIN is 1kHz,
MAX 为 1000GHz.

Example:	FREQ:STAR?	Query the start frequency of sweep measurement.
	FREQ:STAR? MAX	Query the maximum settable start frequency of sweep measurement.
	SENS:FREQ:STAR 8GHz	Set the start frequency of sweep measurement to 8GHz.

Reset state: 1GHz.

[:SENSe[1]:]FREQuency[:CW|FIXed]:STEP

Function: Query or set the frequency step number for the external trigger buffer sweep measurement.

Associated commands:
[:SENSe[1]:]FREQuency[:CW|FIXed]:STARt
[:SENSe[1]:]FREQuency[:CW|FIXed]:STOP
[:SENSe[1]:]BUFFer:COUNt
The number of frequency steps can be 0. When it is 0, the [:SENSe[1]:]BUFFer:COUNt

command can be used to set the buffer measurement size; when it is not 0, the set value of [:SENSe[1]:]BUFFer:COUNt is invalid.

The following equation can be used to calculate the number of frequency steps (Step) (Start, Stop, and Interval are the start frequency, stop frequency and frequency interval respectively. The Interval cannot be 0).

$$Step = (\text{int})\left|\frac{Start - Stop}{Interval}\right| + 1$$

Query: [:SENSe[1]:]FREQuency[:CW|FIXed]:STEP? [MIN|MAX]

Setting: [:SENSe[1]:]FREQuency[:CW|FIXed]:STEP <numeric data>

Valid values for numeric data are: DEF, MIN, MAX, <NRf>, where DEF and <NRf> are used for setting only.

<NRf> ranges from 0 to 80000.

DEF is 0,

MIN is 0,

MAX 为 80000.

Example:

FREQ:STEP?	Query the number of frequency steps.
FREQ:STEP? MAX	Query the maximum settable frequency steps.
SENS:FREQ:STEP 100	Set the number of frequency steps to 100.

Reset state: until 0 is returned.

[:SENSe[1]:]FREQuency[:CW|FIXed]:STOP

Function: Query or set the frequency for the stop frequency of the external trigger buffer sweep measurement.

Associated commands:

[:SENSe[1]:]FREQuency[:CW|FIXed]:STARt

[:SENSe[1]:]FREQuency[:CW|FIXed]:STEP

The start frequency can be greater than or equal to the stop frequency.

Query: [:SENSe[1]:]FREQuency[:CW|FIXed]:STOP? [MIN|MAX]

Setting: [:SENSe[1]:]FREQuency[:CW|FIXed]:STOP <numeric data>

Valid values for numeric data are: DEF, MIN, MAX, <NRf>, where DEF and <NRf> are used for setting only.

<NRf> ranges 1e3 to 1e12, in Hz,

DEF is 1GHz,

MIN is 1kHz,

MAX 为 1000GHz.

Example:

FREQ:STOP?	Query the end frequency of sweep measurement.
FREQ:STOP? MAX	Query the maximum settable stop frequency of sweep measurement.
SENS:FREQ:STOP 8GHz	Set the end frequency of sweep measurement to 8GHz.

Reset state: 1GHz.

[:SENSe[1]:]LIST:FREQuency:STARt

Function: Query or set the start frequency of the timeslot list sweep measurement.

Related commands:

[:SENSe[1]:]LIST:FREQuency:STOP

Query: [:SENSe[1]:]LIST:FREQuency:STARt? [MIN|MAX]

Setting: [:SENSe[1]:]LIST:FREQuency:STARt <numeric data>

Valid values for numeric data are: DEF, MIN, MAX, <NRf>, where DEF and <NRf> are used for setting only.

<NRf> ranges 1e3 to 1e12, in Hz,

DEF is 1GHz,

MIN is 1kHz,

MAX 为 1000GHz.

Example:

LIST:FREQ:STAR?	Query the start frequency of the timeslot list sweep measurement.
LIST:FREQ:STAR? MAX	Query the maximum settable start frequency of the timeslot list sweep measurement.
SENS:LIST:FREQ:STAR 8GHz	Set the start frequency of the timeslot list sweep measurement to 8GHz.

Error message: If the current time timeslot list sweep measurement is in progress, it prompts "-221, "Settings conflict"";

If the detection measurement method (SENS:DET:FUNC) is "AVER", the message "-221, it prompts "Settings conflict"".

Reset state: 1GHz.

[:SENSe[1]:]LIST:FREQuency:STOP

Function: Query or set the stop frequency of the timeslot list sweep measurement.

Related commands:

[:SENSe[1]:]LIST:FREQuency:STARt

Query: [:SENSe[1]:]LIST:FREQuency:STOP? [MIN|MAX]

Setting: [:SENSe[1]:]LIST:FREQuency:STOP <numeric data>

Valid values for numeric data are: DEF, MIN, MAX, <NRf>, where DEF and <NRf> are used for setting only.

<NRf> ranges 1e3 to 1e12, in Hz,

DEF is 1GHz,

MIN is 1kHz,

MAX 为 1000GHz.

Example:

LIST:FREQ:STOP?	Query the stop frequency of the timeslot list sweep measurement.
LIST:FREQ:STOP? MAX	Query the maximum settable stop frequency of the timeslot list sweep measurement.
SENS:LIST:FREQ:STOP 8GHz	Set the stop frequency of the timeslot list

sweep measurement to 8GHz.

Error message: If the current time timeslot list sweep measurement is in progress, it prompts "-221, "Settings conflict"";

If the detection measurement method (SENS:DET:FUNC) is "AVER", the message "-221, it prompts "Settings conflict"".

Reset state: 1GHz.

[:SENSe[1]:]LIST:MTYPe

Function: Query or set the timeslot list sweep measurement type, which is only used for external trigger measurement.

Query: [:SENSe[1]:]LIST:MTYPe?

Setting: [:SENSe[1]:]LIST:MTYPe <string>

<string> can be the following values:

"AVER": average power measurement mode

"PEAK": peak power measurement mode

"PTAV": peak-to-average ratio measurement mode

"MIN": minimum power measurement mode

Example:

LIST:MTYP?	Query the type of the current timeslot list sweep frequency measurement.
SENS:LIST:MTYP "PEAK"	Set the timeslot list sweep measurement type to "Peak".

Error message: If the current time timeslot list sweep measurement is in progress, it prompts "-221, "Settings conflict"";

If the parameter is an invalid string, it prompts "-224, "Illegal parameter value"".

Reset state: Average power measurement mode

[:SENSe[1]:]LIST:POINts

Function: Query or set the number of points for timeslot list sweep measurement, which is only used for external trigger measurement.

If the start frequency (Start) and the stop frequency (Stop) of the slot list sweep are different, then after determining the frequency step (Step), the following equation can be used to calculate the number of measurement points (Points) (Step cannot be zero):

$$Points = (\text{int})\left|\frac{Start - Stop}{\text{Step}}\right| + 1$$

Query: [:SENSe[1]:]LIST:POINts? [MIN|MAX]

Setting: [:SENSe[1]:]LIST:POINts <numeric data>

Valid values for numeric data are: DEF, MIN, MAX, <NRf>, where DEF and <NRf> are used for setting only.

<NRf> ranges from 1 to 5000.

DEF is 1,

MIN is 1,

MAX 为 5000.

Example:	LIST:POIN?	Query the number of points of the timeslot list sweep measurement.
	LIST:POIN? MAX	Query the maximum settable points of the timeslot list sweep measurement.
	SENS:LIST:POIN 100	Set the number of points for the timeslot list sweep measurement to 100.

Error message: If the current time timeslot list sweep measurement is in progress, it prompts "-221, "Settings conflict"";
If the detection measurement method (SENS:DET:FUNC) is "AVER", the message "-221, it prompts "Settings conflict"".

Reset state: until 1 is returned.

[:SENSe[1]:]LIST:STATe

Function: Query or set the timeslot list sweep measurement state.

Query: [:SENSe[1]:]LIST:STATe?

Setting: [:SENSe[1]:]LIST:STATe <Boolean data>
Valid forms of <Boolean data> are: 0, OFF, 1, ON


Example:	LIST:STAT?	Query the timeslot list sweep measurement state.
	LIST:STAT 1	Enable the timeslot list sweep measurement

Error message: If the current time timeslot list sweep measurement is in progress, it prompts "-221, "Settings conflict"";
If the detection measurement method (SENS:DET:FUNC) is "AVER", it prompts "-221, "Settings conflict"";
If the trigger source (TRIG:SOUR) is not "external trigger", it prompts "-221, "Settings conflict"".

Reset state: Off

[:SENSe[1]:]LIST:TSCount

Function: Query or set the number of slots for the timeslot list sweep measurement.
The timeslot diagram is shown below:

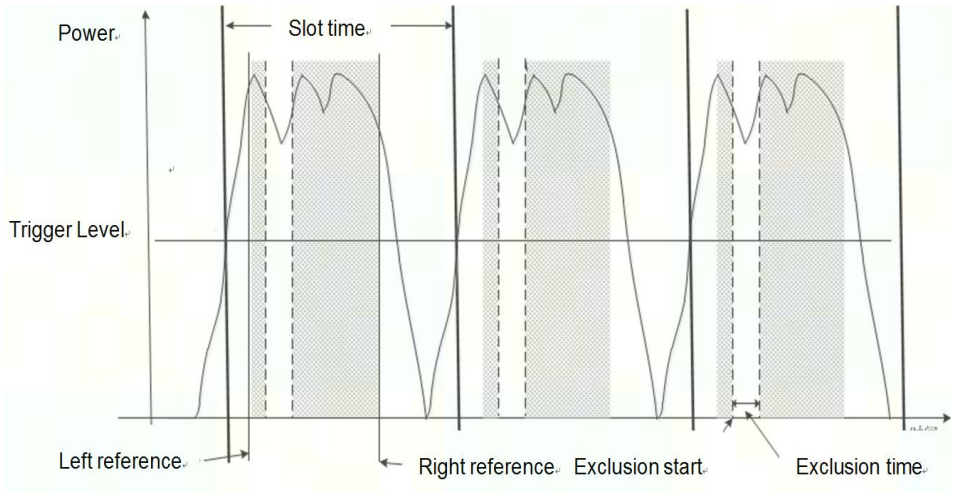

Query: [:SENSe[1]:]LIST:TSCount? [MIN|MAX]

Setting: [:SENSe[1]:]LIST:TSCount <numeric data>

Valid values for numeric data are: DEF, MIN, MAX, <NRf>, where DEF and <NRf> are used for setting only.

<NRf> ranges from 1 to 16.

DEF is 1,

MIN is 1,

MAX 为 16.

Example:

LIST:TSC?	Query the number of time slots for the timeslot list sweep measurement.
LIST:TSC? MAX	Query the maximum settable time slots for the timeslot list sweep measurement.
SENS:LIST:TSC 8	Set the number of time slots for the timeslot list sweep measurement to 8.

Error message: If the current time timeslot list sweep measurement is in progress, it prompts "-221, "Settings conflict"";

If the detection measurement method (SENS:DET:FUNC) is "AVER", it prompts "-221, "Settings conflict"";

If the product of the time length of the timeslot measurement (LIST:TSL:TIME) and the number of time slots (LIST:TSC) exceeds 1s, it prompts "-221, "Settings conflict"".

Reset state: until 1 is returned.

Description: The number of measurement points returned by FETCh?, MEASure?, READ? is the number of sweep measurement points multiplied by the number of time slots. For example, if the number of measurement points is 100 and the number of time slots is 8, then the above command returns 800 measurements each time.

[:SENSe[1]:]LIST:TSLot:EXCLude:OFFSet:TIME

Function: Query or set the start time (offset time) of the "measurement exclusion area" relative to the start position of the slot (see "Exclusion Start" in the slot diagram).

Query: [:SENSe[1]:]LIST:TSLot:EXCLude:OFFSet:TIME? [MIN|MAX]

Setting: [:SENSe[1]:]LIST:TSLot:EXCLude:OFFSet:TIME <numeric data>

Valid values for numeric data are: DEF, MIN, MAX, <NRf>, where DEF and <NRf> are used for setting only.

<NRf> ranges from 0 to 0.1, in seconds with an accuracy of 12.5ns

DEF is 0,

MIN is 0,

MAX 为 0.1.

Example:

LIST:TSL:EXCL:OFFS:TIME?	Query the start time of "measurement exclusion area".
LIST:TSL:EXCL:OFFS:TIME? MAX	Query the maximum settable start time of "measurement exclusion area".
LIST:TSL:EXCL:OFFS:TIME 1e-5	Set the start time of "measurement exclusion area" to 10us.

Error message: If the current time timeslot list sweep measurement is in progress, it prompts "-221, "Settings conflict"";

If the detection measurement method (SENS:DET:FUNC) is "AVER", the message "-221, it prompts "Settings conflict"".

Reset state: 0s.

[:SENSe[1]:]LIST:TSLot:EXCLude:TIME

Function: Query or set the time duration of the "measurement exclusion area" relative to the start position of the slot (see "Exclusion Duration" in the slot diagram).

Query: [:SENSe[1]:]LIST:TSLot:EXCLude:TIME? [MIN|MAX]

Setting: [:SENSe[1]:]LIST:TSLot:EXCLude:TIME <numeric data>

Valid values for numeric data are: DEF, MIN, MAX, <NRf>, where DEF and <NRf> are used for setting only.

<NRf> ranges from 0 to 0.1, in seconds with an accuracy of 12.5ns

DEF is 0,

MIN is 0,

MAX 为 0.1.

Example:

LIST:TSL:EXCL:TIME?	Query the time duration of "measurement exclusion area".
LIST:TSL:EXCL:TIME? MAX	Query the maximum settable time duration of "measurement exclusion area".
LIST:TSL:EXCL:TIME 1e-5	Set the time duration of "measurement exclusion area" to 10us.

Error message: If the current time timeslot list sweep measurement is in progress, it prompts "-221, "Settings conflict"";

If the detection measurement method (SENS:DET:FUNC) is "AVER", the message "-221, it prompts "Settings conflict"".

Reset state: 0s.

3.3 Instrument Subsystem Command

[:SENSe[1]:]LIST:TSLot:TIME

Function: Query or set the time duration of the timeslot measurement (see "Time Slot Duration" in the slot diagram).

Query: [:SENSe[1]:]LIST:TSLot:TIME? [MIN|MAX]

Setting: [:SENSe[1]:]LIST:TSLot:TIME <numeric data>

Valid values for numeric data are: DEF, MIN, MAX, <NRf>, where DEF and <NRf> are used for setting only.

<NRf> ranges from 12.5e-9 to 1, in seconds with an accuracy of 12.5ns

DEF is 1e-4,

MIN is 12.5e-9,

MAX 为 1.

Example:

LIST:TSL:TIME?	Query the time duration of timeslot measurement.
LIST:TSL:TIME? MAX	Set the time span of time domain measurement Query the maximum settable time slot measurement length.
LIST:TSL:TIME 1e-3	Set the time slot measurement length to 1ms.

Error message: If the current time timeslot list sweep measurement is in progress, it prompts "-221, "Settings conflict"";

If the detection measurement method (SENS:DET:FUNC) is "AVER", it prompts "-221, "Settings conflict"";

If the product of the time length of the timeslot measurement (LIST:TSL:TIME) and the number of time slots (LIST:TSC) exceeds 1s, it prompts "-221, "Settings conflict"".

Reset state: 100us.

[:SENSe[1]:]LIST:TSLot:TREF[1]|2

Function: Query or set the left and right reference values (percentage relative to the slot duration) of the timeslot measurement gate (see "Left reference" and "Right reference" in the slot diagram), TREF1: left reference, TREF2: right reference.

The left reference value is defined as the percentage of the start time of the measurement gate divided by the time slot length, and the right reference value is defined as the difference between the time slot end time and the end time of the measurement gate divided by the time slot length.

This function effectively removes rising and falling edges and overshoot of the signal.

Note: The sum of the left and right reference values shall not exceed 100 (in %).

Query: [:SENSe[1]:]LIST:TSLot:TREF[1]|2? [MIN|MAX]

Setting: [:SENSe[1]:]LIST:TSLot:TREF[1]|2 <numeric data>

Valid values for numeric data are: DEF, MIN, MAX, <NRf>, where DEF and <NRf> are used for setting only.

<NRf> ranges from 0 to 100, in PCT,
DEF is 0,
MIN is 0,
MAX 为 100.

Example:	LIST:TSL:TREF1?	Query the left reference value of the timeslot measurement gate.
	LIST:TSL:TREF2? MAX	Query the right reference value of the maximum settable timeslot measurement gate.
	LIST:TSL:TREF2 10	Set the left reference value of the timeslot measurement gate to 10%.

Error message: If the current time timeslot list sweep measurement is in progress, it prompts "-221, "Settings conflict"";
If the detection measurement method (SENS:DET:FUNC) is "AVER", the message "-221, it prompts "Settings conflict"".

Reset state: until 0 is returned.

[:SENSe[1]:]MRATe

Function: Query or set the measurement speed.

Query: [:SENSe[1]:]MRATe?

Setting: [:SENSe[1]:]MRATe <character data>
The valid values of the character data are as follows:
NORMal or 0: 20 readings per second at normal speed
DOUBle or 1: 40 readings per second at doubled speed
FAST or 2: 50000 readings per second at fast speed (the detector measurement method (SENS:DET:FUNC) is "AVER")
Note: In the fast test mode, the following setting parameters are ignored and processed by "OFF": average state, channel offset state, measurement offset state, relative measurement state, and limit state.

Example:	MRAT?	Query the measurement speed
	SENS:MRAT FAST	Set the quick measurement

Reset state: Normal speed

[:SENSe[1]:]POWer:AC:RANGe

Function: Query or set the range of the sensor(total 4 rangs).
When the range is set with this command, the automatic range status will be changed to manual,
namely, set [SENSe[1]]|SENSe2:POWer:AC:RANGe:AUTO to OFF.

Query: [:SENSe[1]|2]:POWer:AC:RANGe?

Setting: [:SENSe[1]|2]:POWer:AC:RANGe <0|1|2|3>

Example:	SENS:POW:AC:RANG?	Query the range of the sensor.

POW:AC:RANG 1 Set the range of the sensor to 1.

Limit: None

Reset state: None

Error message: None

[:SENSe[1]:]POWer:AC:RANGe:AUTO

Function: Query or set the automatic range switch state of the sensor.
When the automatic range is enabled, the power meter will automatically adjust the range according to the power signal, and adopt the optimal range for measurement
Relevant command:
[:SENSe[1]|2]:POWer:AC:RANGe。

Query: [:SENSe[1]|2]:POWer:AC:RANGe:AUTO?

Setting: [:SENSe[1]|2]:POWer:AC:RANGe:AUTO <Boolean data>
Valid forms of <Boolean data> are: 0, OFF, 1, ON

Example: SENS:POW:AC:RANG:AUTO? Query the automatic range switch of sensor.
POW:AC:RANG:AUTO 0 Disable the automatic range of sensor.

Limit: None

Reset state: None

Error message: ON

[:SENSe[1]:]SWEep:APERture

Function: Query or set the measurement aperture or measurement time interval.
The relevant command is: [:SENSe[1]:]SWEep:APERture:AUTO
After the measurement aperture is set, the auto-measurement aperture state is set to OFF.

Query: [:SENSe[1]:]SWEep:APERture? [MIN|MAX]

Setting: [:SENSe[1]:]SWEep:APERture <numeric data>
Valid values for numeric data are: DEF, MIN, MAX, <NRf>, where DEF and <NRf> are used for setting only.
<NRf> ranges from 20e-6 to 1, in seconds.
DEF is 50ms,
MIN is 20us,
MAX 为 1s.

Example: SENS:SWE:APER? Query the current measured aperture.
SWE:APER 1e-3 Set the measurement aperture to 1ms

Limit: It can be set only when the trigger source is set to IMMediate

Reset state: OFF

Error message: None

[:SENSe[1]:]SWEep:APERture:AUTO

Function: Query or set the auto-measurement aperture or measurement interval state.

If it is set to auto-measurement aperture, the measured aperture value will be automatically selected according to the measurement speed, and the corresponding relationship is as follows:

Normal measurement speed, with an aperture of 50ms;

Doubled measurement speed with an aperture of 25ms;

Fast measurement speed with an aperture of 20us ((SENS:DET:FUNC) for "AVER");

with an aperture of 20us ((SENS:DET:FUNC) for "NORM");

Query: [:SENSe[1]:]SWEep:APERture:AUTO

Setting: [:SENSe[1]:]SWEep:APERture:AUTO <Boolean data>

Valid forms of <Boolean data> are: 0, OFF, 1, ON

Example:

SENS:SWE:APER:AUTO?	Query the current auto-measurement aperture state.
SWE:APER:AUTO 1	Set to auto-measurement aperture

Limit: None

Reset state: 50ms

Error message: None

3.3.8 Status Subsystem Command (STATus)

The Status subsystem command detects the status of the 87235 by monitoring the Device Status Register, the Operational Status Register, and the Questionable Question Register.

- :STATus:DEVice:CONDition?.....112
- :STATus:DEVice:ENABle.....112
- :STATus:DEVice[:EVENt]?.....112
- :STATus:DEVice:NTRansition.....112
- :STATus:DEVice:PTRansition.....113
- :STATus:OPERation:CALibrating[:SUMMary]:CONDition?.....113
- :STATus:OPERation:CALibrating[:SUMMary]:ENABle.....113
- :STATus:OPERation:CALibrating[:SUMMary][:EVENt]?.....113
- :STATus:OPERation:CALibrating[:SUMMary]:NTRansition.....114
- :STATus:OPERation:CALibrating[:SUMMary]:PTRansition.....114
- :STATus:OPERation:CONDition?.....114
- :STATus:OPERation:ENABle.....115

3.3 Instrument Subsystem Command

- :STATus:OPERation[:EVENt]?.....115
- :STATus:OPERation:NTRansition.....115
- :STATus:OPERation:PTRansition.....115
- :STATus:OPERation:LLFail[:SUMMary]:CONDition?.....116
- :STATus:OPERation:LLFail[:SUMMary]:ENABle.....116
- :STATus:OPERation:LLFail[:SUMMary][:EVENt]?.....116
- :STATus:OPERation:LLFail[:SUMMary]:NTRansition.....117
- :STATus:OPERation:LLFail[:SUMMary]:PTRansition.....117
- :STATus:OPERation:SENSe[:SUMMary]:CONDition?.....117
- :STATus:OPERation:SENSe[:SUMMary]:ENABle.....117
- :STATus:OPERation:SENSe[:SUMMary][:EVENt]?.....118
- :STATus:OPERation:SENSe[:SUMMary]:NTRansition.....118
- :STATus:OPERation:SENSe[:SUMMary]:PTRansition.....118
- :STATus:OPERation:TRIGger[:SUMMary]:CONDition?.....119
- :STATus:OPERation:TRIGger[:SUMMary]:ENABle.....119
- :STATus:OPERation:TRIGger[:SUMMary][:EVENt]?.....119
- :STATus:OPERation:TRIGger[:SUMMary]:NTRansition.....119
- :STATus:OPERation:TRIGger[:SUMMary]:PTRansition.....120
- :STATus:OPERation:ULFail[:SUMMary]:CONDition?.....120
- :STATus:OPERation:ULFail[:SUMMary]:ENABle.....120
- :STATus:OPERation:ULFail[:SUMMary][:EVENt]?.....121
- :STATus:OPERation:ULFail[:SUMMary]:NTRansition.....121
- :STATus:OPERation:ULFail[:SUMMary]:PTRansition.....121
- :STATus:PRESet.....122
- :STATus:QUEStionable:CALibration[:SUMMary]:CONDition?.....122
- :STATus:QUEStionable:CALibration[:SUMMary]:ENABle.....122
- :STATus:QUEStionable:CALibration[:SUMMary][:EVENt]?.....123
- :STATus:QUEStionable:CALibration[:SUMMary]:NTRansition.....123
- :STATus:QUEStionable:CALibration[:SUMMary]:PTRansition.....123
- :STATus:QUEStionable:CONDition?.....123
- :STATus:QUEStionable:ENABle.....124
- :STATus:QUEStionable[:EVENt]?.....124
- :STATus:QUEStionable:NTRansition.....124
- :STATus:QUEStionable:PTRansition.....125

- :STATus:QUEStionable:POWer[:SUMMary]:CONDition?.....125
- :STATus:QUEStionable:POWer[:SUMMary]:ENABle.....125
- :STATus:QUEStionable:POWer[:SUMMary][:EVENt]?.....126
- :STATus:QUEStionable:POWer[:SUMMary]:NTRansition.....126
- :STATus:QUEStionable:POWer[:SUMMary]:PTRansition.....126

Table 3.10 Commands or events affecting the status register

Status Register	*RST	*CLS	Start up	STATus:PRESet
SCPI transition filter (NTR and PTR)	No effect	No effect	Preset	Preset
SCPI enable register	No effect	No effect	Preset	Preset
SCPI event register	No effect	Clear	Clear	No effect
SCPI error/event queue enable	No effect	No effect	Preset	Preset
SCPI error/event queue	No effect	Clear	Clear	No effect
IEEE488.2 Register ESE SRE	No effect	No effect	Clear	No effect
IEEE488.2 Register SESR STB	No effect	Clear	Clear	No effect

Preset status description: The preset value of PTR is 0x7fff (32767); both NTR and enable registers are cleared.

- Command Sets.....93
- Transition Filter.....94
- Device Status Register Description.....95
- Operation Status Register Description.....97
- Calibration Operation Status Register Description.....98
- Lower Limit Detection Operation Status Register Description.....99
- Sensing Operation Status Register Description.....101
- Question Status Register Description.....105
- Calibration Question Status Register Description.....107
- Power Question Status Register Description.....109

3.3.10.1 Command Sets

The content of the state register can be queried or set with the following command set:

:CONDition?

Query the value of the condition register of the state register. The return format is < NR1 > . The range is from 0 to 32767. After the query, the value of the condition register remains unchanged.

:ENABle <NRf>|<non-decimal number>

3.3 Instrument Subsystem Command

Query or set the event enable register of the state register, and the highest bit (bit15) is always 0.

[:EVENt?]

Query the event register of the state register, and clear the register after the query.

:NTRansition <NRf>|<non-decimal number>

Query or set the negative transition filter of the state register, and the highest bit is always 0.

:PTRansition <NRf>|<non-decimal number>。

Query or set the positive transition filter of the state register, and the highest bit is always 0.

The status registers supported in this case are

STATus:DEVice

STATus:OPERation

STATus:OPERation:CALibrating[:SUMMary]

STATus:OPERation:LLFail[:SUMMary]

STATus:OPERation:SENSe[:SUMMary]

STATus:OPERation:TRIGger[:SUMMary]

STATus:OPERation:ULFail[:SUMMary]

STATus:QUEStionable

STATus:QUEStionable

STATus:QUEStionable:CALibration[:SUMMary]

STATus:QUEStionable:POWer[:SUMMary]

For example:

:CONDition?can be used to query the calibration operation registerSTATus:OPERation:CALibrating[:SUMMary]

STATus:OPERation:CALibrating[:SUMMary]:CONDition?

The :ENABle can be used to query or set the calibration operation register STATus:OPERation:CALibrating[:SUMMary]

STATus:OPERation:CALibrating[:SUMMary]:ENABle

3.3.10.2 Transition Filter

Refer to Section 9.2 of SCPI-99 for a description of the transition filter. A brief description is given below.

1) Positive transition (PTR): When the condition is set to TRUE by the FALSE event.

2) Negative transition (NTR): When the condition goes from TRUE to FALSE, the event is set to TRUE.

3) Positive transition or negative transition: The event is set to TRUE when the condition goes from FALSE to TRUE or TRUE to FALSE.

4) Clearing the positive transition and negative transition registers will disable event reporting.

3.3.10.3 Device Status Register Description (STATus:DEVice)

Table 3.11 Device Status Register Description

Bit	Value	Definition
0	1	Unused
1	2	Channel A detection state
2	4	Channel B detection state (for dual-channel only)
3	8	Channel A error state
4	16	Channel B error state (for dual-channel only)
5	32	USB channel detection state (reserved)
6	64	USB channel error state (reserved)
7--14	-	Unused
15	-	Always 0

1) Bits 1 and 2 indicate the detection state of Channel A and Channel B, respectively.

a) Return value of STATus:DEVice:CONDition?: 1 indicates that it is detected, and 0 indicates that it is not detected.

b) Return value of STATus:DEVice[:EVENt]?: 1 indicates that a connection or removal event has occurred. 0 means not occurred. After the query, the event register will be cleared.

c) When STATus:DEVice:NTRansition is set to 1, STATus:DEVice[:EVENt] will be set to 1 if shiftis detected.

d) When STATus:DEVice:PTRansition is set to 1, STATus:DEVice[:EVENt] will be set to 1 if access is detected.

2) Bits 3 and 4 indicate errors for Channel A and Channel B of the 87235, respectively. 1 means error, and 0 means no error found.

3.3 Instrument Subsystem Command

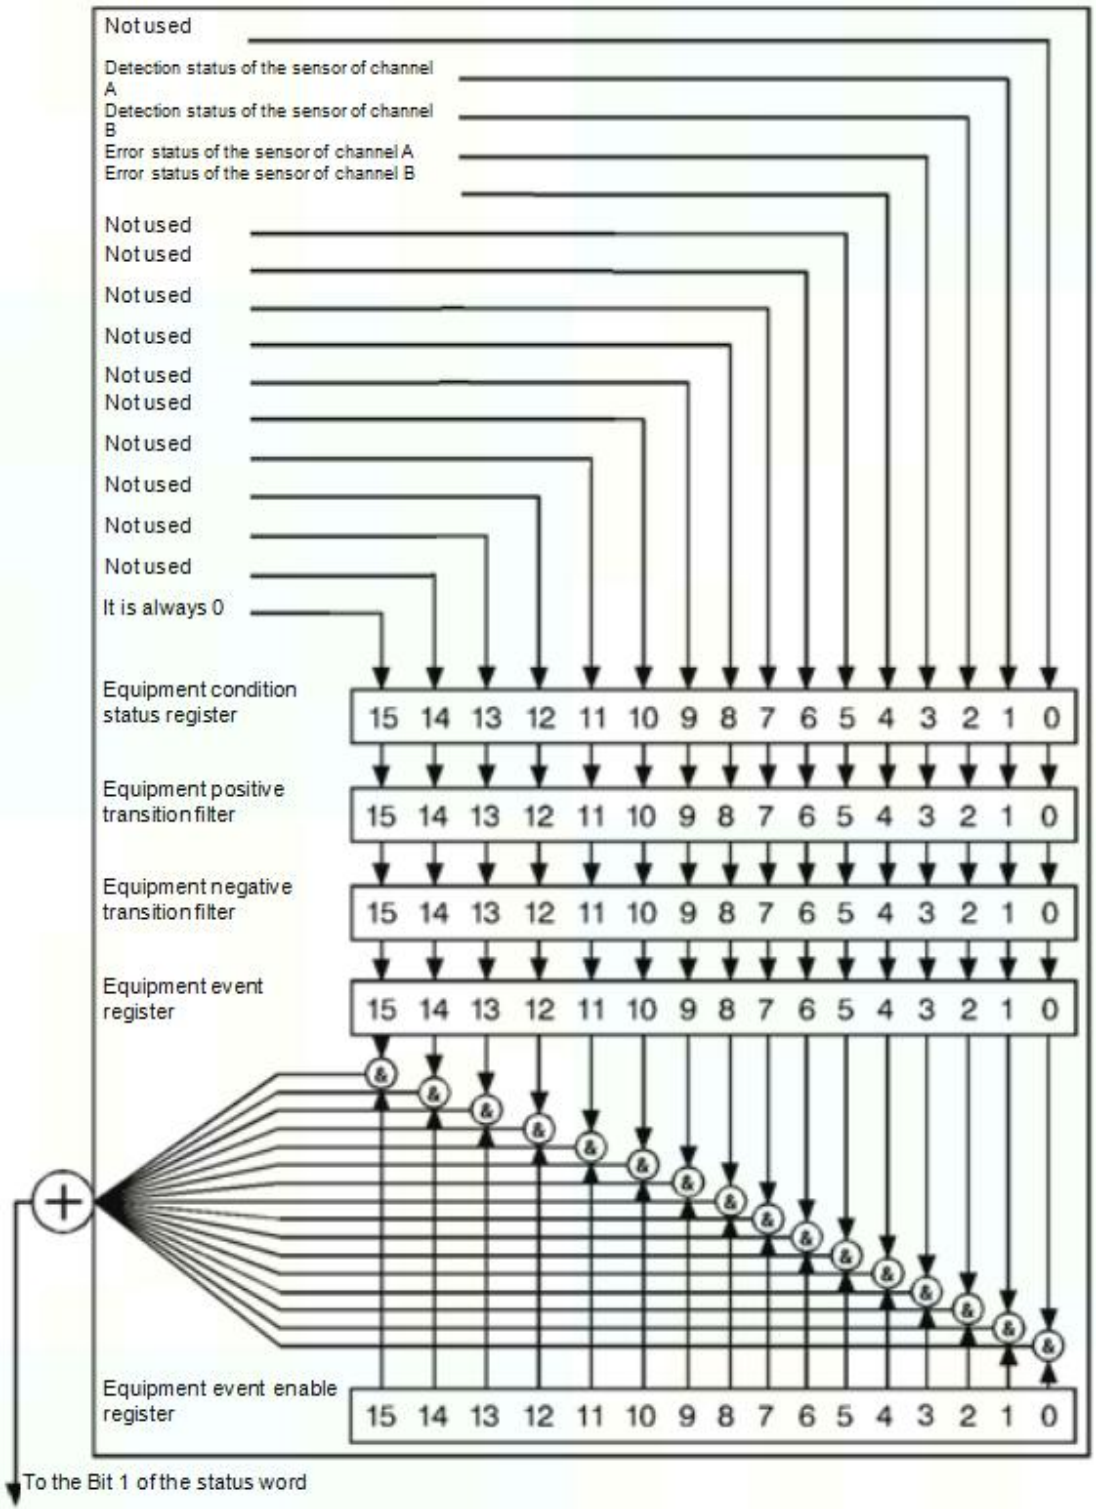


Figure 3.5 Device status register

3.3.10.4 Operation Status Register Description (STATus:OPERation)

Table 3.12 Operation status register description

Bit	Value	Definition
0	1	Calibration Summary
1--4	-	Unused
5	32	Wait for Trigger Summary
6--9	-	Unused
10	1024	Sensing Summary
11	2048	Lower-Limit Detection Failure Summary (LLF)
12	4096	Upper-Limit Detection Failure Summary (ULF)
13--14	-	Unused
15	-	Always 0

Six groups of operation registers are included:

STATus:OPERation

STATus:OPERation:CALibrating[:SUMMary]

STATus:OPERation:LLFail[:SUMMary]

STATus:OPERation:SENSe[:SUMMary]

STATus:OPERation:TRIGger[:SUMMary]

STATus:OPERation:ULFail[:SUMMary]

3.3 Instrument Subsystem Command

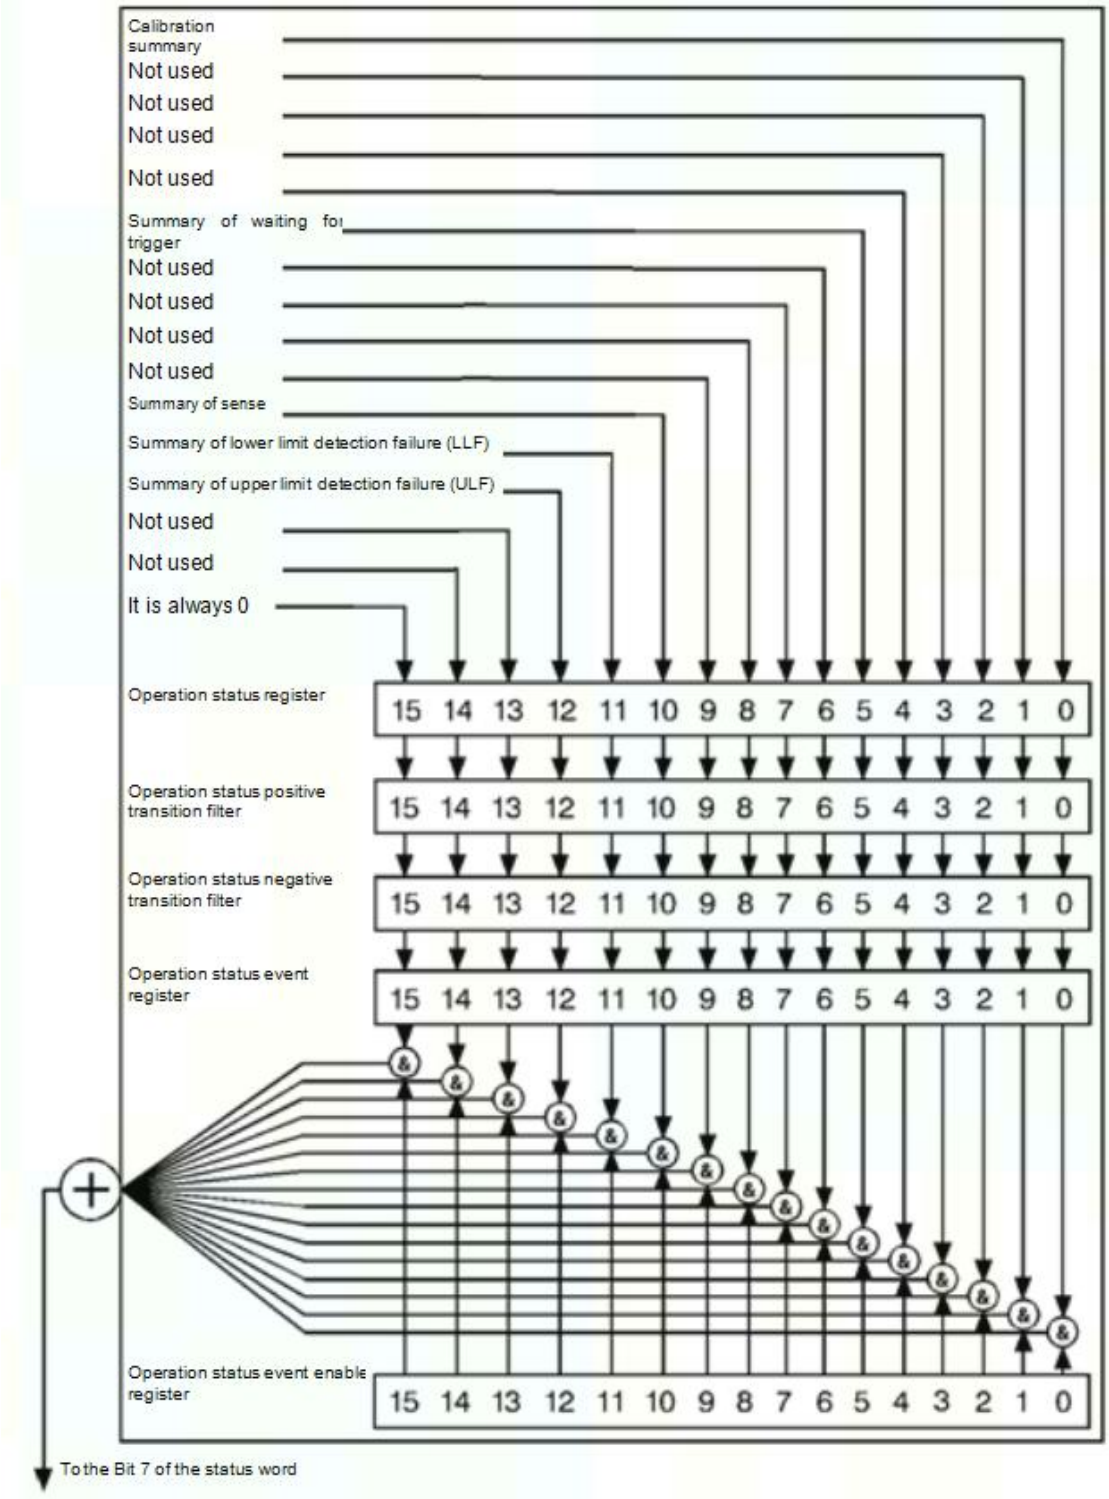


Figure 3.6 Operation status register description

3.3.10.5 Calibration Operation Status Register Description (STATus:OPERation:CALibrating[:SUMMary])

Table 3.13 Calibration Operation Status Register Description

Bit	Value	Definition
0	1	Unused
1	2	Channel A calibration status.
2	4	Channel B calibration status. (for dual-channel only)
3--14	-	Unused
15	-	Always 0

Bit 1 and bit 2 indicate the calibration status of Channel A and Channel B respectively. 1 indicates that it is being zeroed or calibrated, and 0 indicates that the calibration is completed or not zeroed or calibrated.

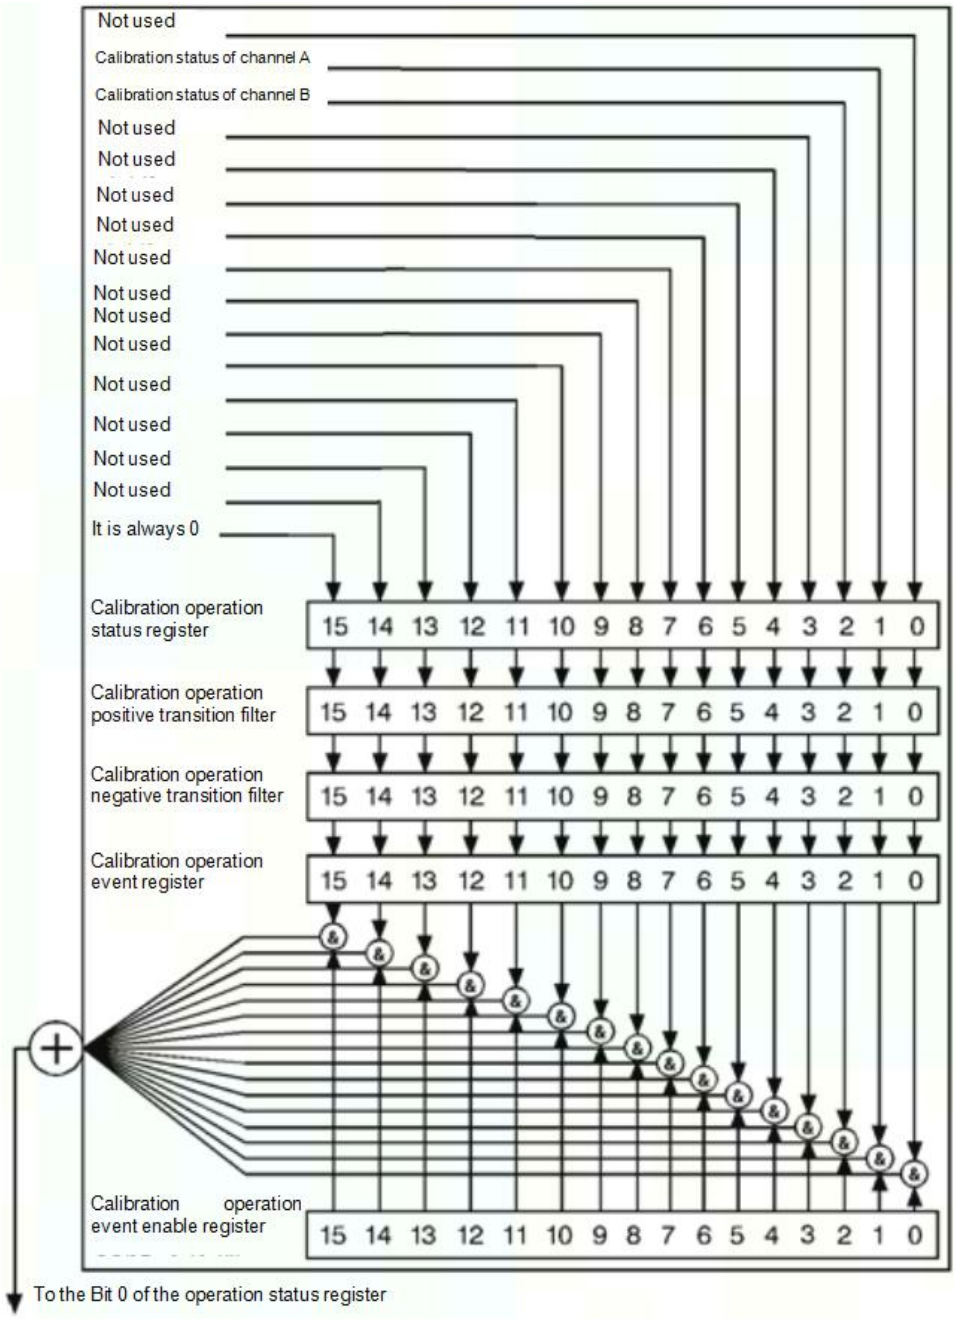


Figure 3.7 Calibration operation status register

3.3.10.6 Lower Limit Status Register Description (STATus:OPERation:CALibrating[:SUMMary])

Table 3.14 Lower Limit Detection Operation Status Register Description

Bit	Value	Definition
0--2	-	Unused
3	8	Lower limit detection state of Measurement 1
4	16	Lower limit detection state of Measurement 2
5	32	Lower limit detection state of Measurement 3
6	64	Lower limit detection state of Measurement 4
7--14	-	Unused
15	-	Always 0

Bit 3 to bit 6 indicates the lower limit failure detection status of the corresponding measurement. 1 indicates that the lower limit is exceeded

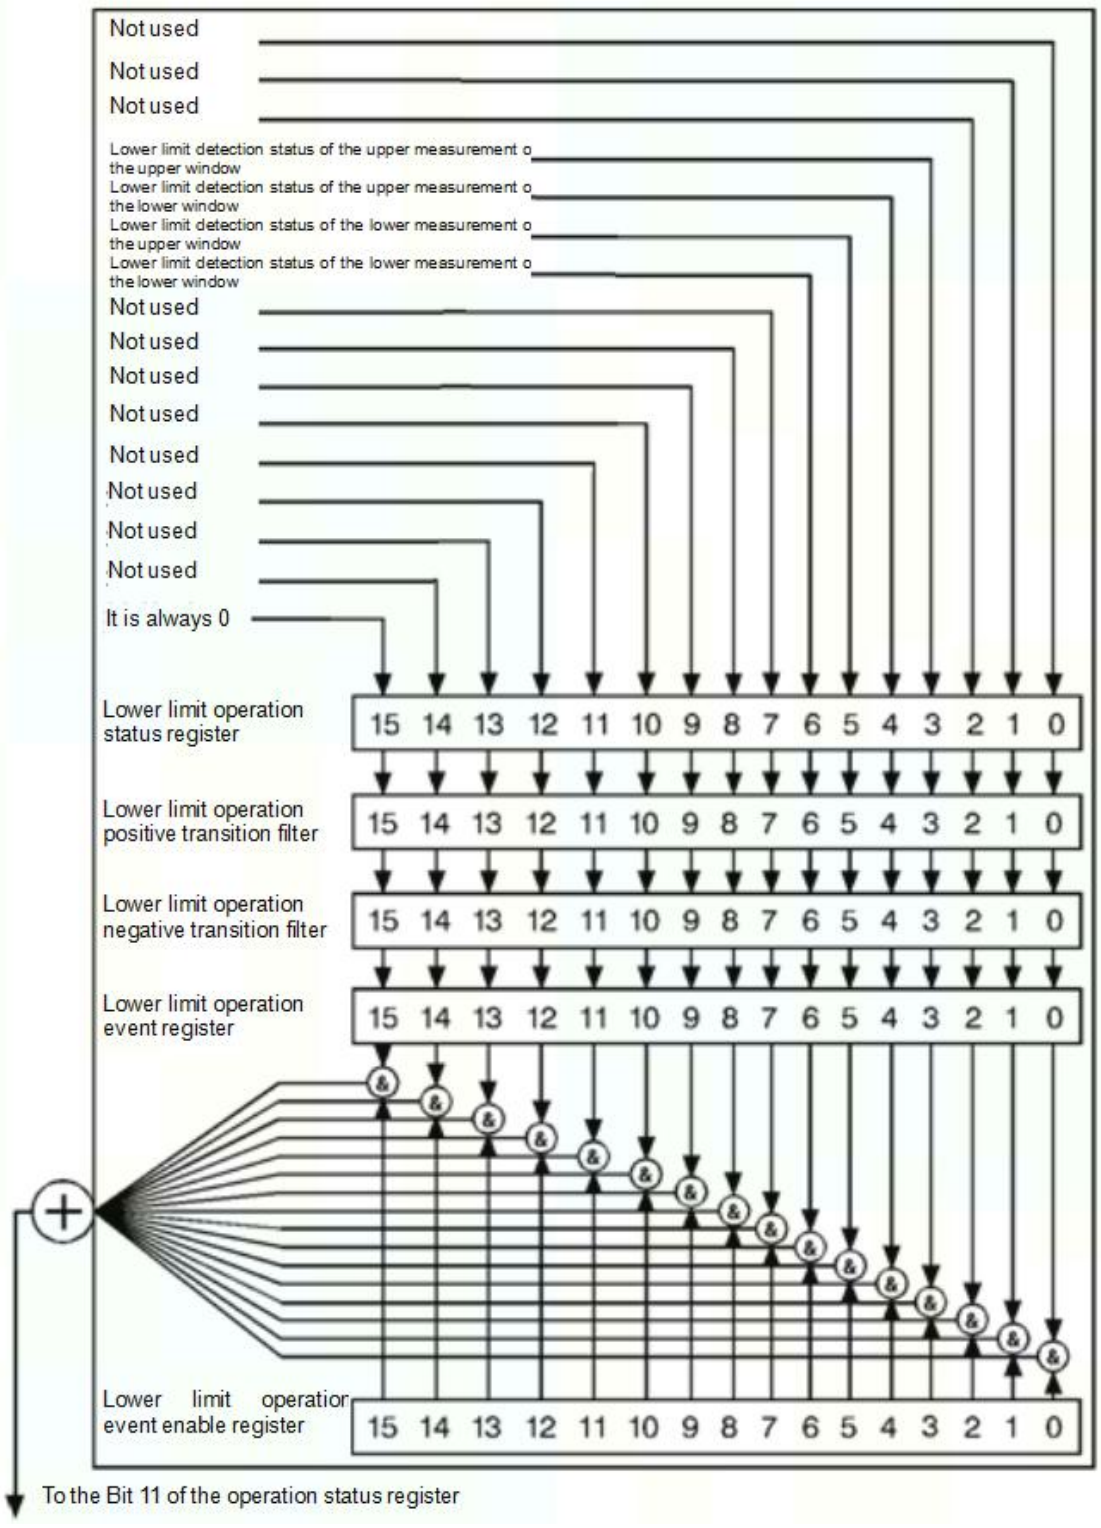


Table 3.8 Lower limit detection operation status register

3.3.10.7 Sensing Operation Status Register Description (STATus:OPERation:SENSe[:SUMMary])

Table 3.15 Sensing operation status register description

Bit	Value	Definition
0	1	Unused
1	2	Channel A reads EEPROM status
2	4	Channel B reads EEPROM status (for dual-channel only)
3--14	-	Unused
15	-	Always 0

Bits 1 and 2 indicate that Channel A and Channel B read EEPROM status, respectively, and 1 indicates that the 87235 is being read.

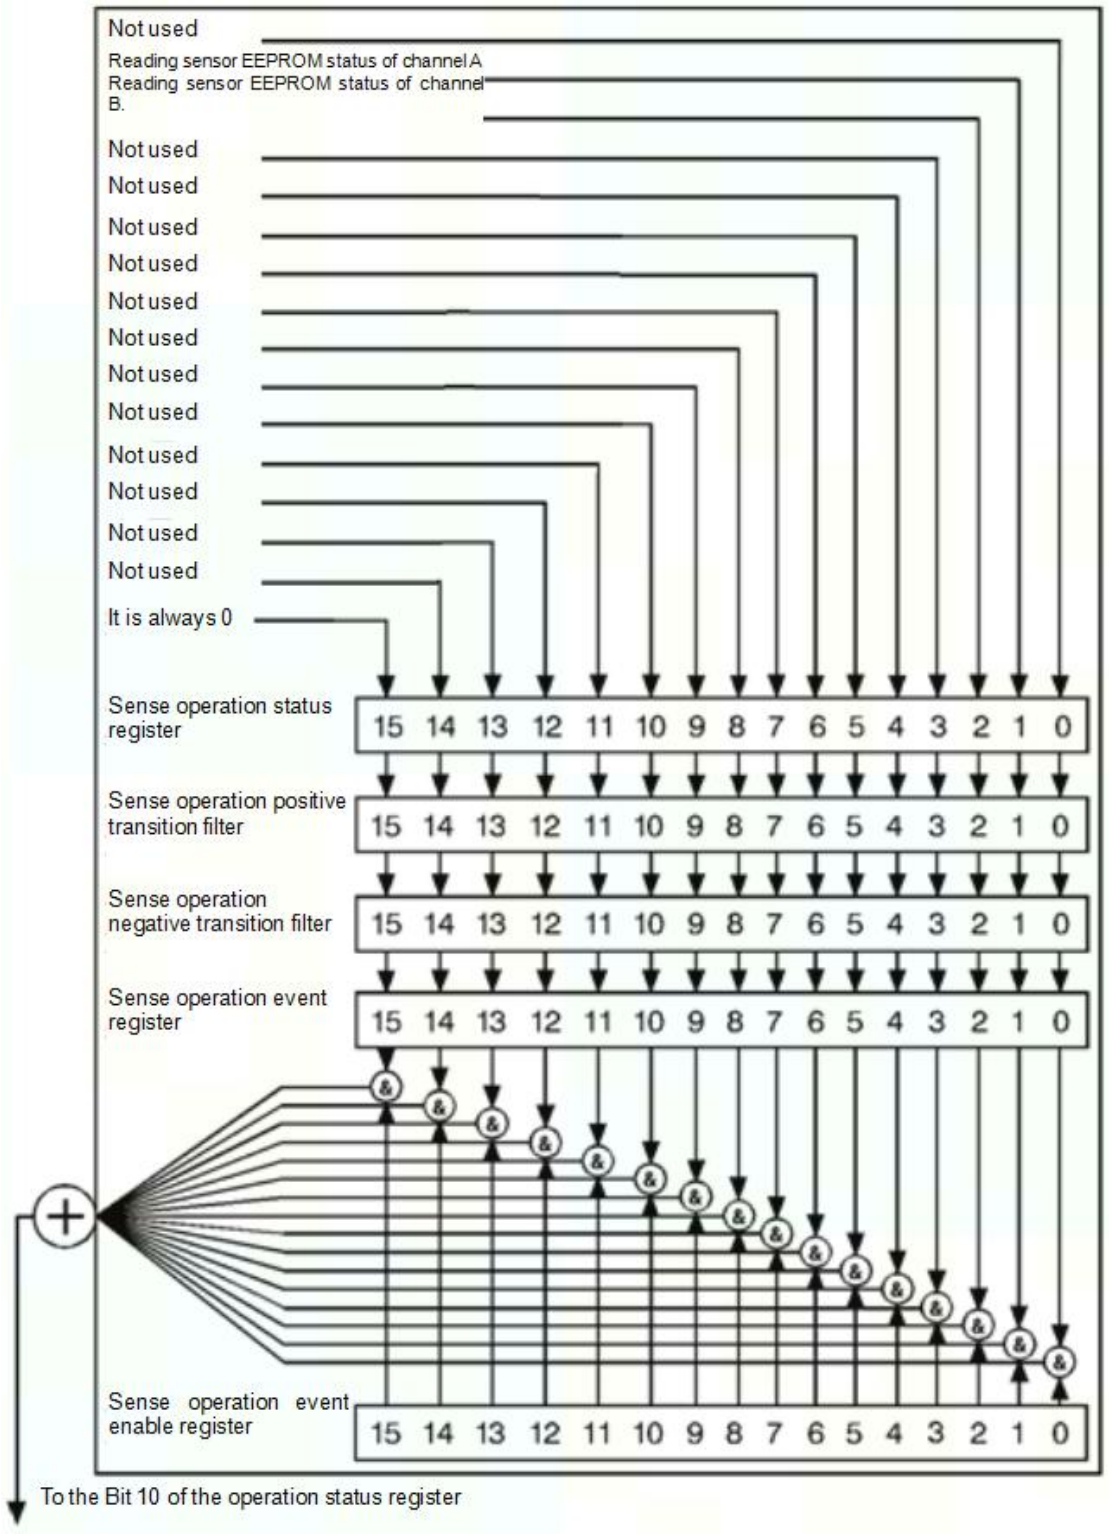


Table 3.9 Sense operation event enable register

3.3 Instrument Subsystem Command

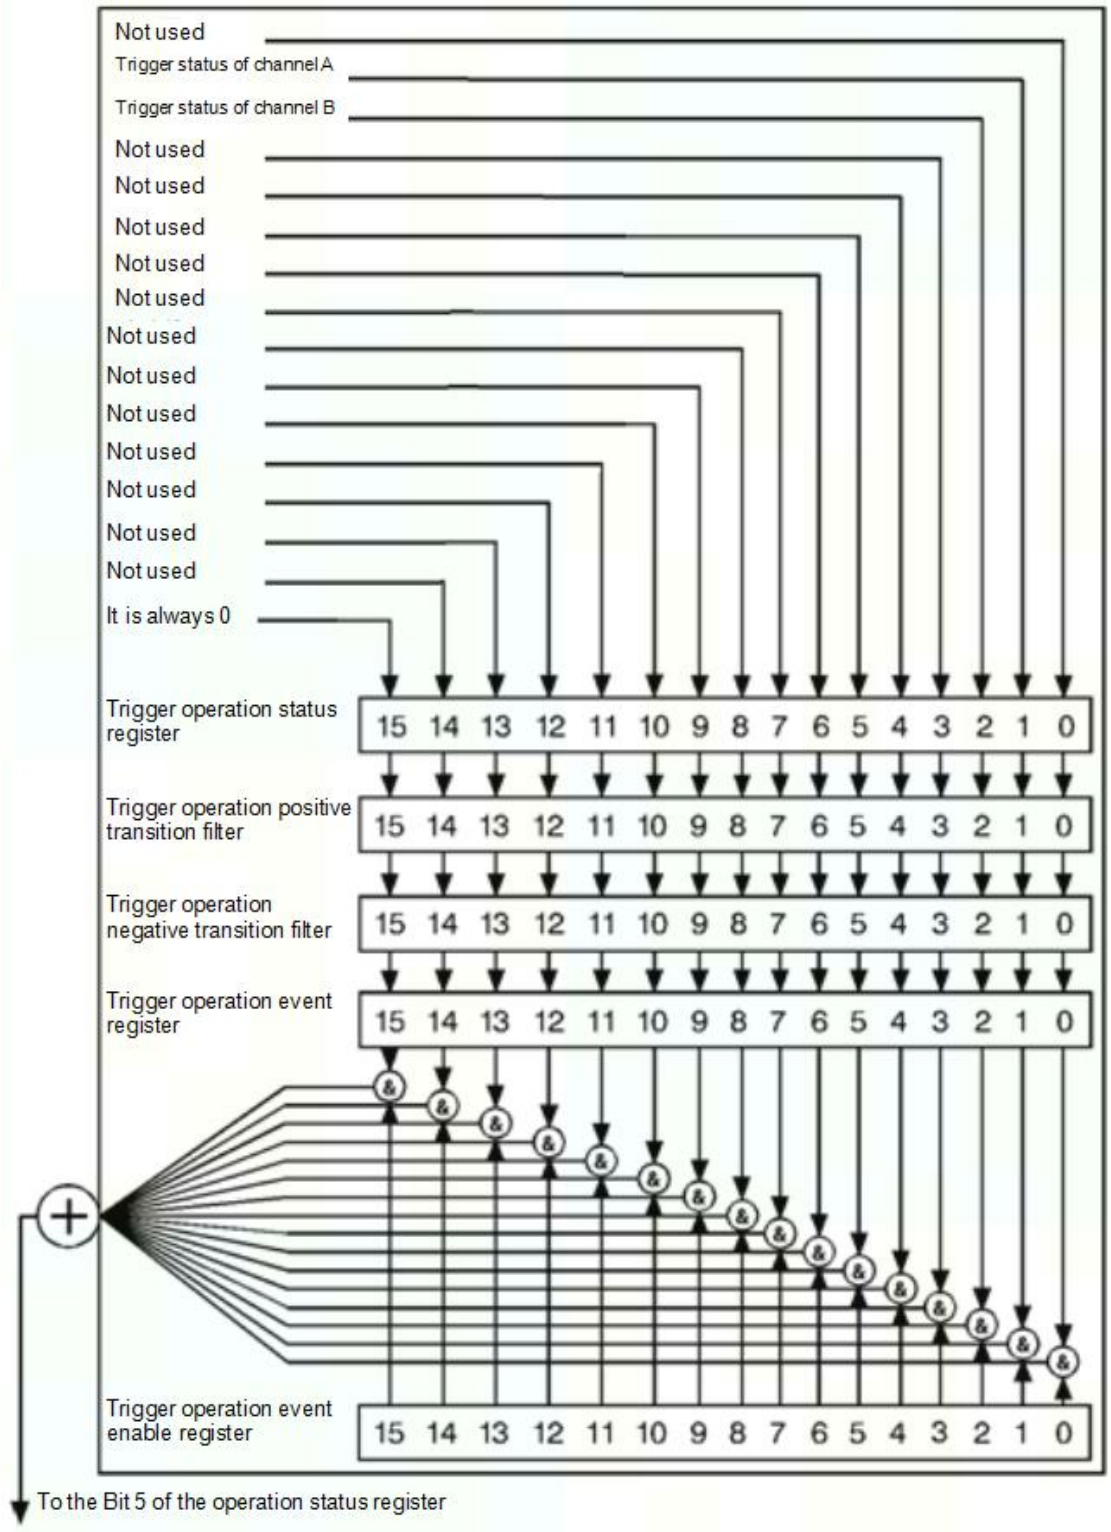


Table 3.10 Trigger operation event enable register

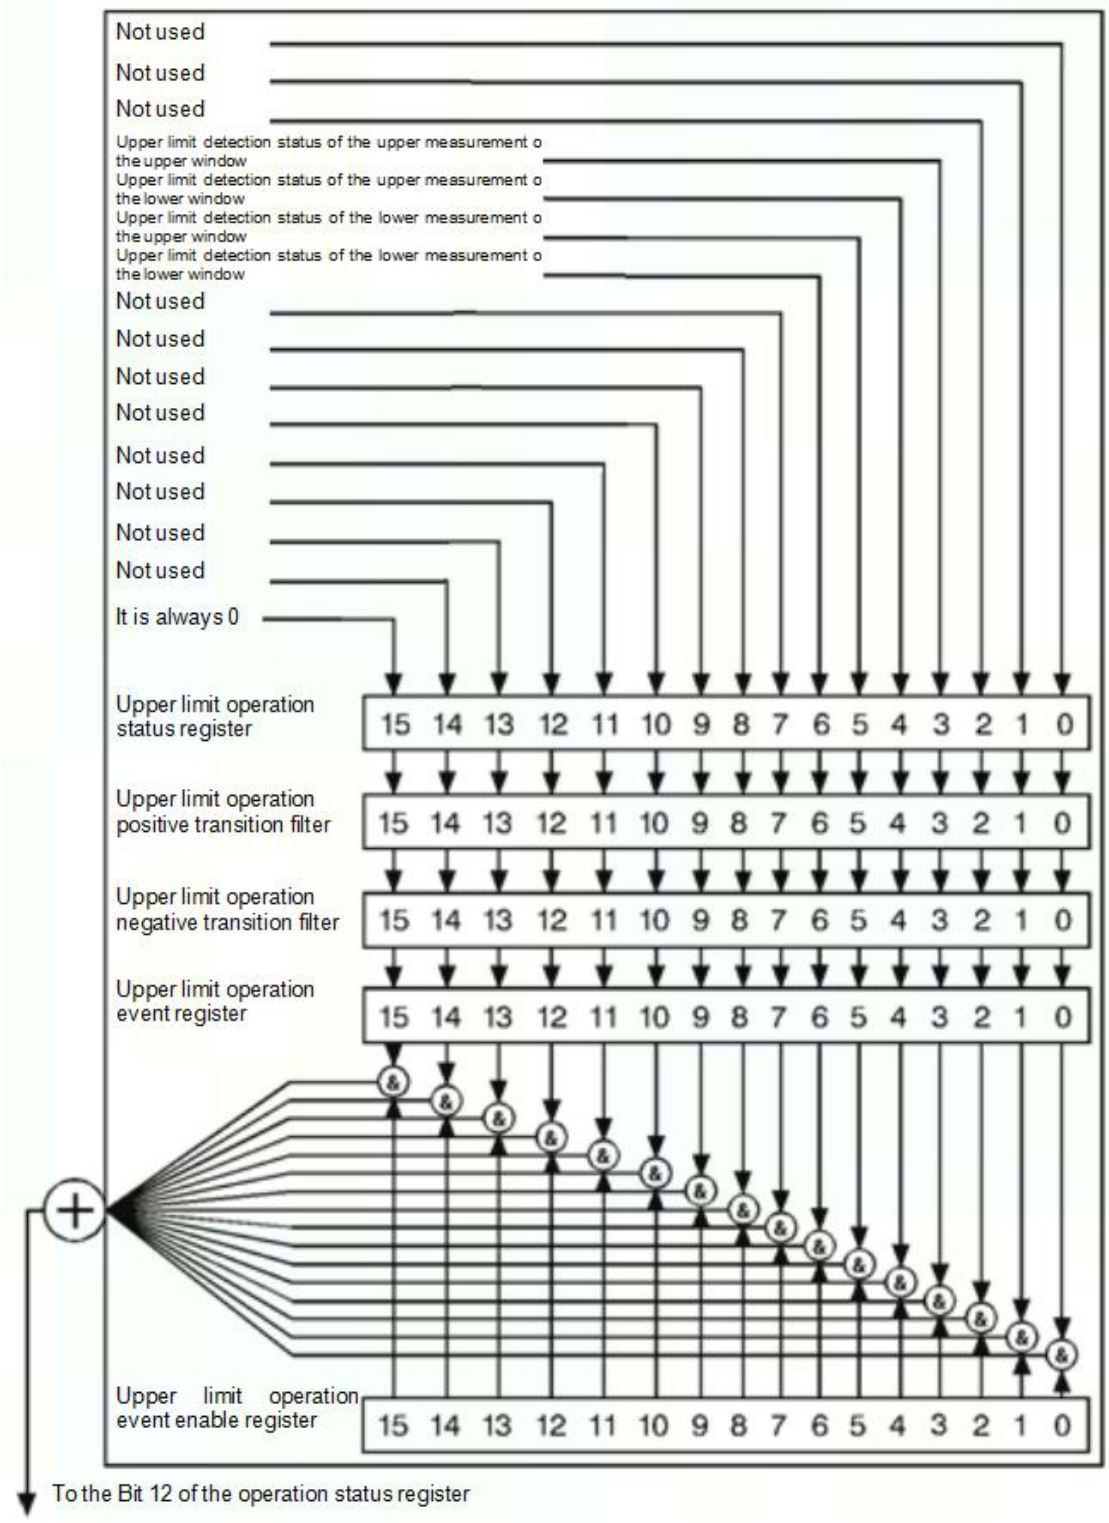


Table 3.11 Upper limit detection operation status register

3.3.10.8 Question Status Register Description (STATus: QUEStionable)

Table 3.18 Question Status Register Description

Bit	Value	Definition
0--2	-	Unused
3	8	Power Summary
4--7	-	Unused
8	256	Calibration Summary
9	512	Power-on self-test
10--14	-	Unused
15	-	Always 0

Three groups of operation registers are included:

STATus:QUEStionable

STATus:QUEStionable:Power[:SUMMary]

STATus:QUEStionable:CALibration[:SUMMary]

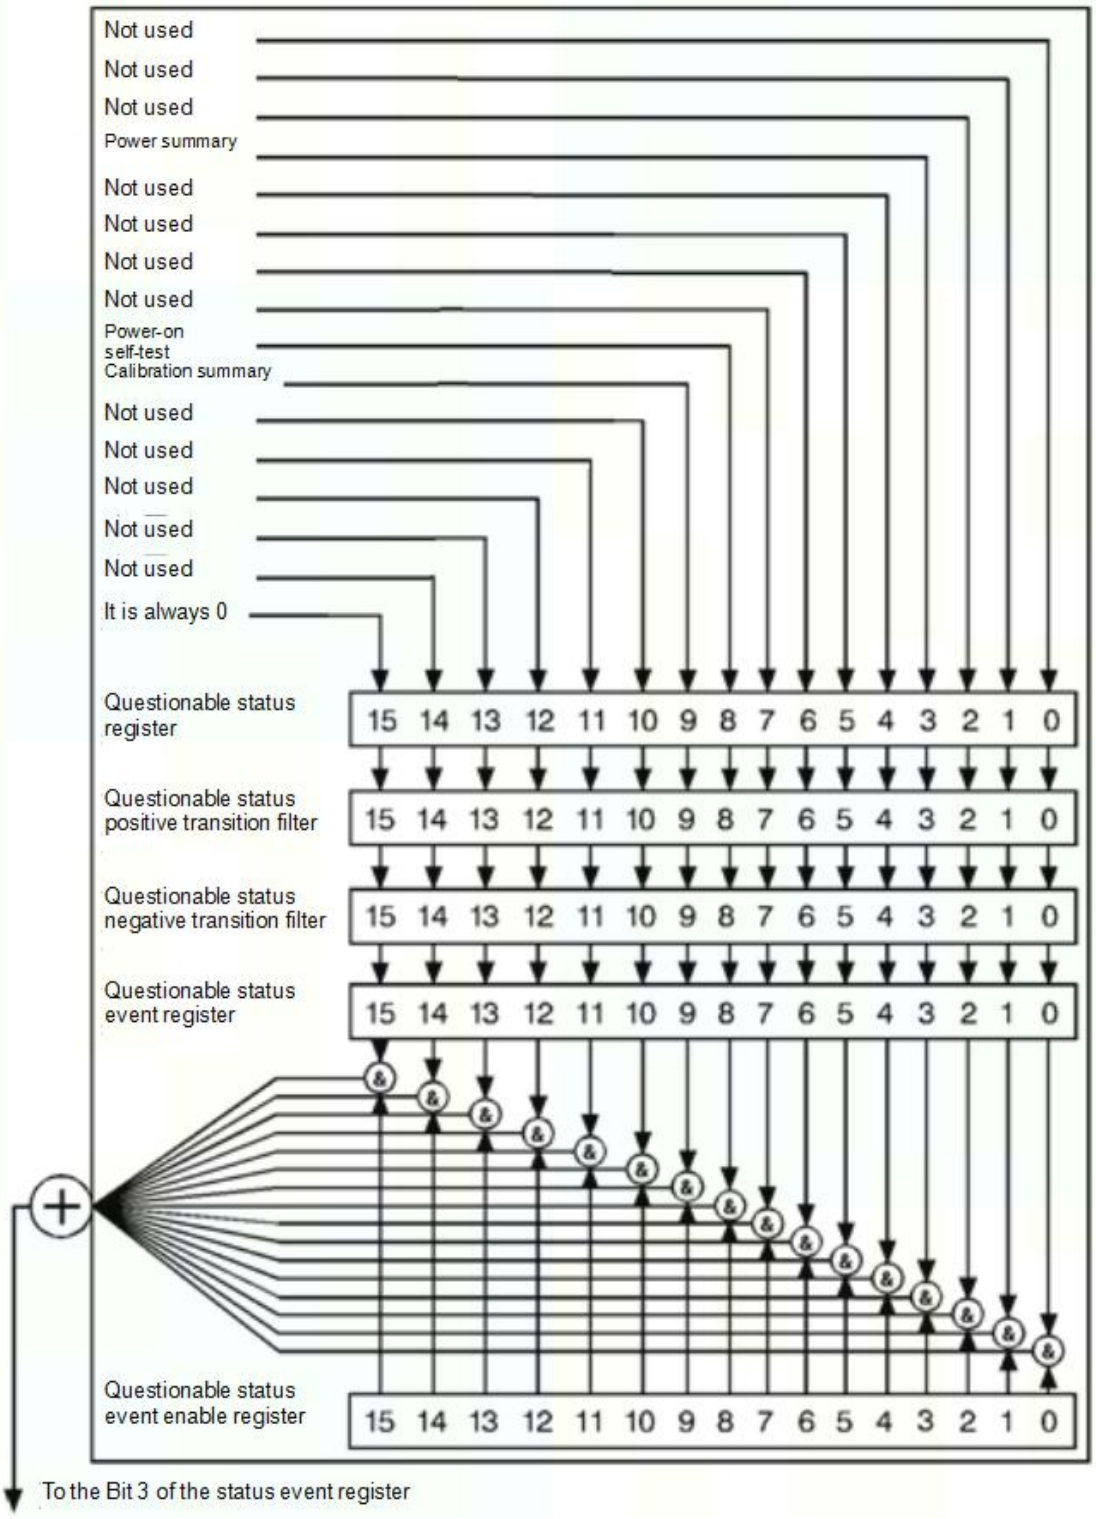


Figure 3.12 Question status register

3.3.10.9 Calibration Question Operation Status Register Description (STATus QUEStionable:CALibrating[:SUMMary])

Table 3.19 Question Status Register Description

Bit	Value	Definition
0	1	Unused
1	2	Channel A zeroing and calibration error
2	4	Channel B zeroing and calibration error (for dual-channel only)
3--14	-	Unused
15	-	Always 0

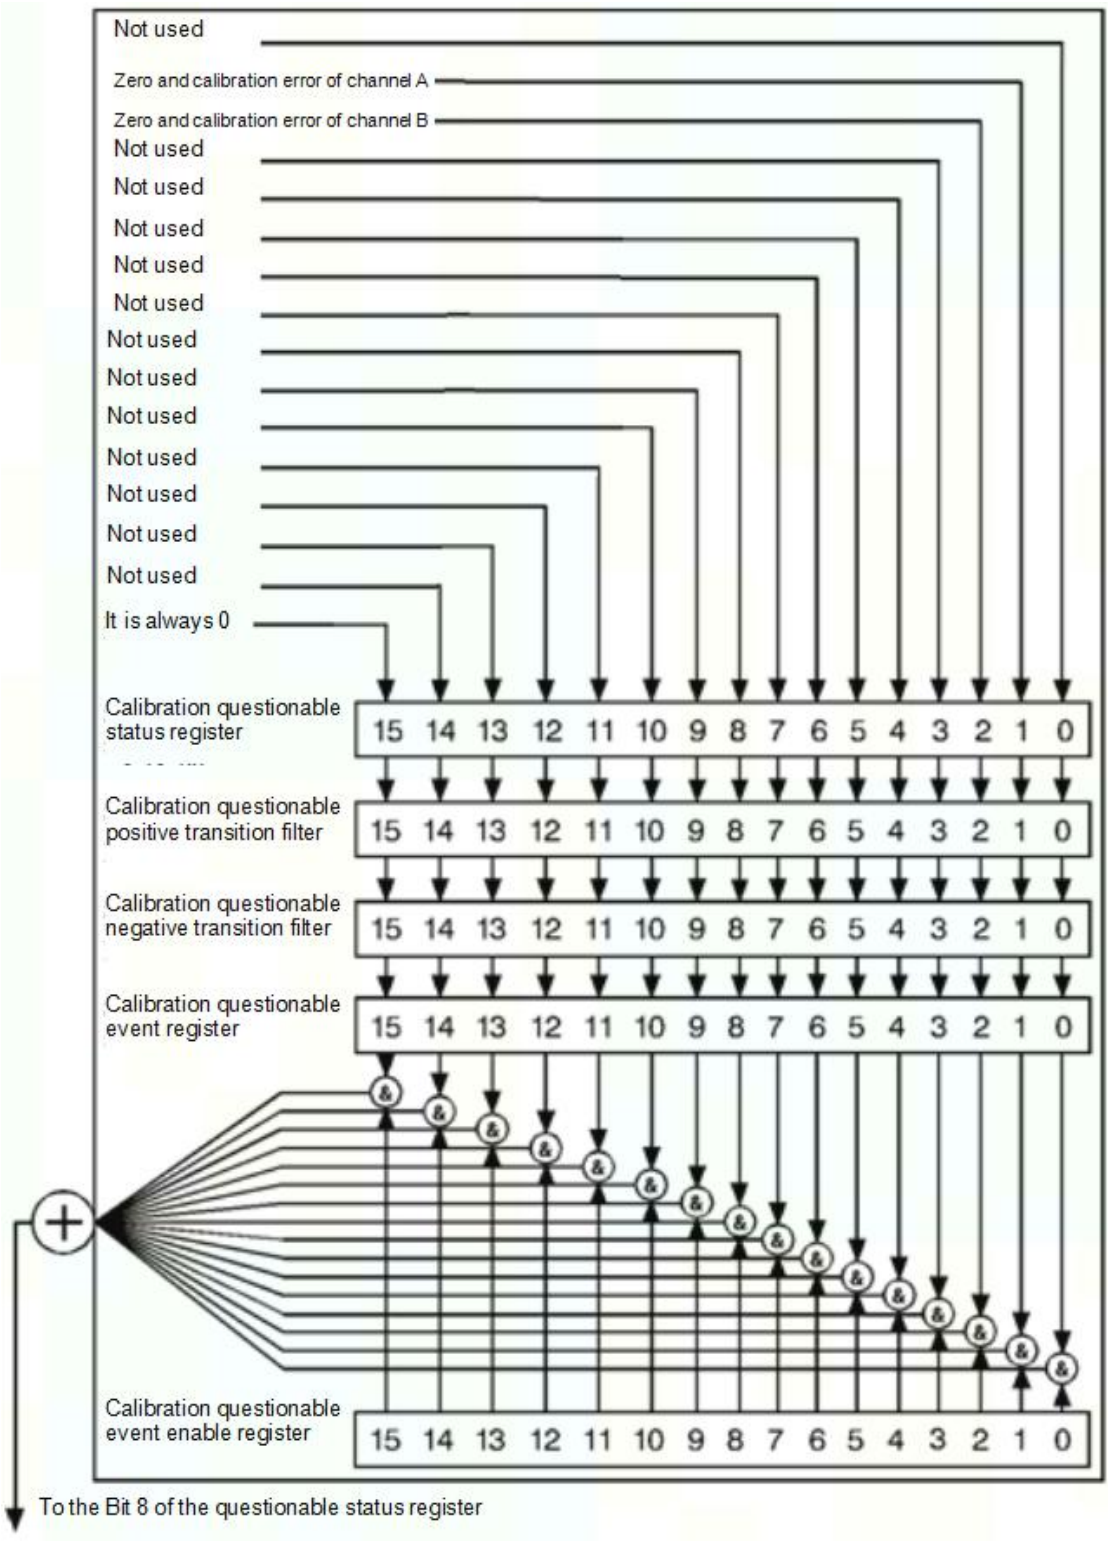


Figure 3.13 Calibration question status register

3.3.10.10 Power Question Status Register Description (STATus:QUEStionable:POWer[:SUMMary])

Table 3.20 Power Question Status Register Description

Bit	Value	Definition
0	1	Unused
1	2	Channel A input is overloaded
2	4	Channel B input overload (for dual-channel only)
3	8	Channel A needs to be zeroed
4	16	Channel B needs to be zeroed (for dual-channel only)
5	32	Measurement 1 data is invalid, or logarithmically incorrect
6	64	Measurement 2 data is invalid, or logarithmically incorrect
7	128	Measurement 3 data is invalid, or logarithmically incorrect
8	256	Measurement 4 data is invalid, or logarithmically incorrect
9--14	-	Unused
15	-	Always 0

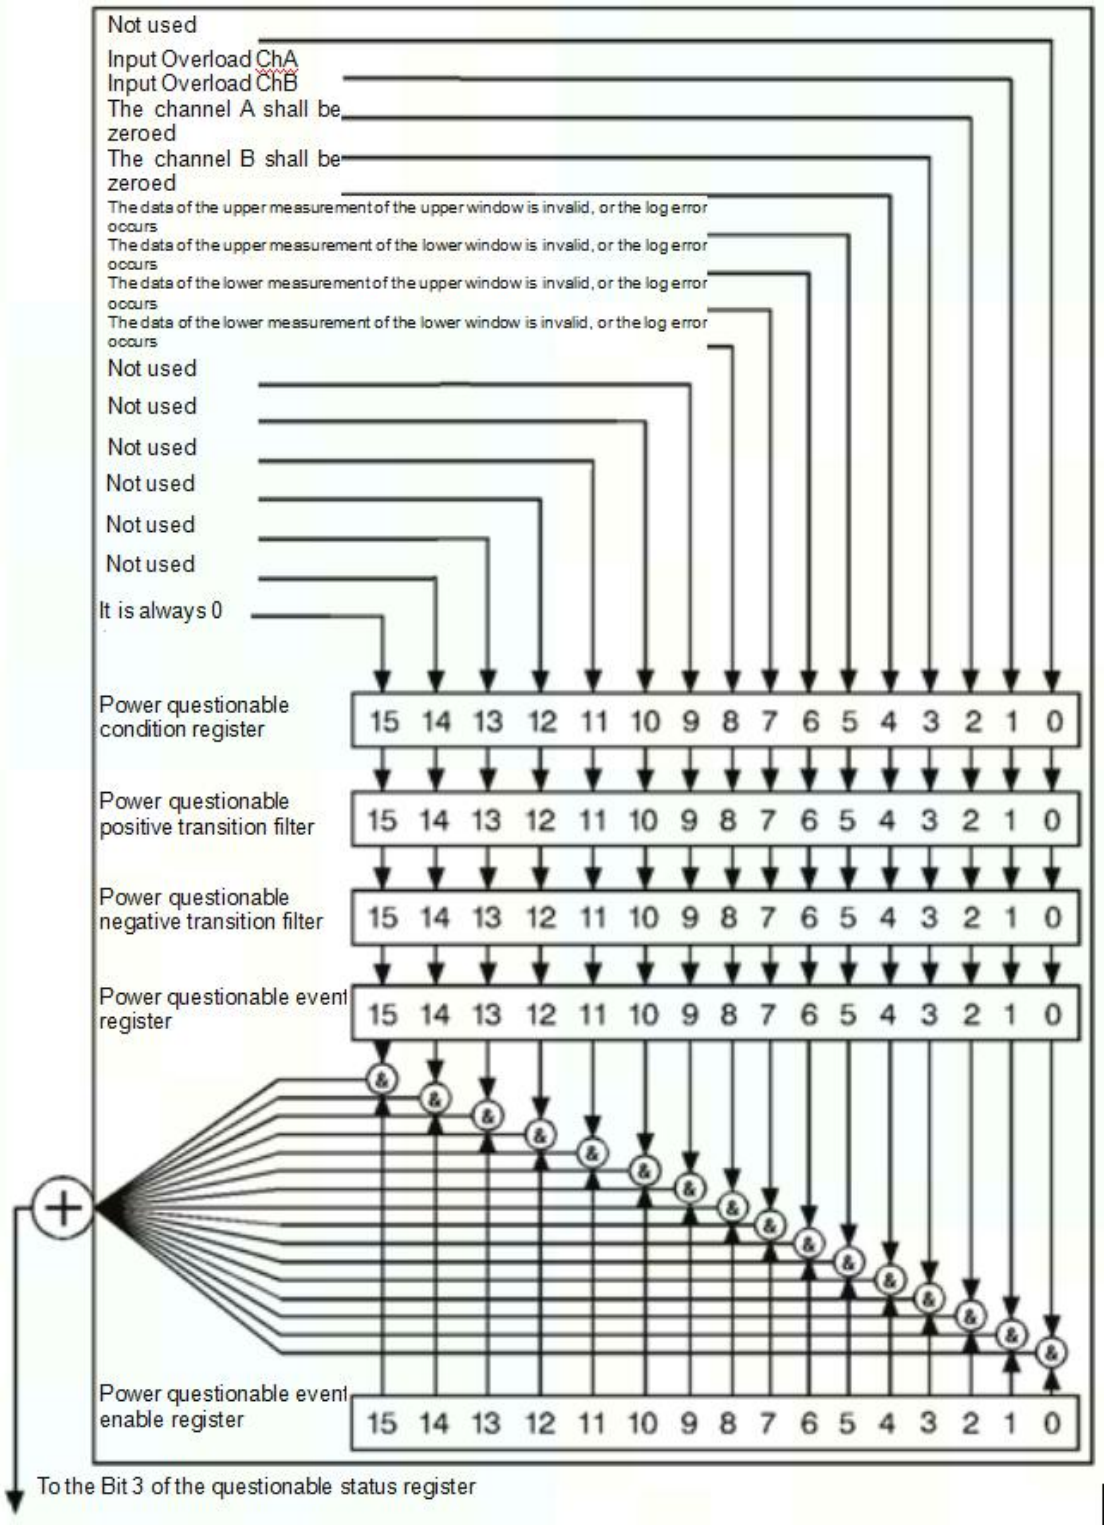


Figure 3.14 Power question status register

3.3 Instrument Subsystem Command

:STATus:DEVice:CONDition?

Function: Query the value in the device status condition register.

Query: :STATus:DEVice:CONDition?

Setting: Not supported

Example: STAT:DEV:COND?

:STATus:DEVice:ENABle

Function: Query or set the device status event enable register. Operate by bit. 0 means that reporting status events to bit 1 (Bit1) of the higher level status word is disabled. 1 indicates enable.

Query: :STATus:DEVice:ENABle?

Setting: :STATus:DEVice:ENABle <NRf>|<non-decimal number>
The parameter range is from 0 to 32767.

Example:

STAT:DEV:ENAB?	Query the device status event enable register.
STAT:DEV:ENAB 6	Enable bit 1 and bit 2, which allows reporting of the 87235 detection events to the status word.
STAT:DEV:ENAB #B0110	The meaning is the same as above, using binary numbers.
STAT:DEV:ENAB #H06	The meaning is the same as above, using hexadecimal numbers.

:STATus:DEVice[:EVENt]?

Function: Query the device event register. After the query, 87235 automatically clears the register.

Query: :STATus:DEVice[:EVENt]?

Setting: Not supported

Example: STAT:DEV?

:STATus:DEVice:NTRansition

Function: Query or set the negative transition filter of the device.

Query: :STATus:DEVice:NTRansition?

Setting: :STATus:DEVice:NTRansition <NRf>|<non-decimal number>
The parameter range is from 0 to 32767.

Example: STAT:DEV:NTR?

STAT:DEV:NTR #H06	Negative transition filters the status of bit 1 and bit 2 into the event register.
STAT:DEV:NTR #B0110	The meaning is the same as above, using binary numbers.
STAT:DEV:NTR 6	The meaning is the same as above, using decimal numbers.

:STATus:DEVice:PTRansition

Function: Query or set the positive transition filter of the device.

Query: :STATus:DEVice:PTRansition?

Setting: :STATus:DEVice:PTRansition <NRf>|<non-decimal number>
The parameter range is from 0 to 32767.

Example: STAT:DEV:PTR?

STAT:DEV:PTR #H06	Positive transition filters the status of bit 1 and bit 2 into the event register.
STAT:DEV:PTR #B0110	The meaning is the same as above, using binary numbers.
STAT:DEV:PTR 6	The meaning is the same as above, using decimal numbers.

:STATus:OPERation:CALibrating[:SUMMary]:CONDition?

Function: Query the value in the calibration operation status condition register.
In the return value, if bit 1 is non-zero, it indicates that Channel A is being zeroed or calibrated; if bit 2 is non-zero, it indicates that Channel B is being zeroed or calibrated. For example, returning 2 indicates that Channel A is being zeroed or calibrated.

Query: :STATus:OPERation:CALibrating[:SUMMary]:CONDition?

Setting: Not supported

Example: STAT:OPER:CAL:COND?

:STATus:OPERation:CALibrating[:SUMMary]:ENABle

Function: Query or set the calibration operation event enable register. Operate by bit. 0 means that reporting of status events to bit 0 (Bit0) of the operation status is disabled. 1 indicates enable.

Query: :STATus:OPERation:CALibrating[:SUMMary]:ENABle?

Setting: :STATus:OPERation:CALibrating[:SUMMary]:ENABle <NRf>|<non-decimal number>
The parameter range is from 0 to 32767.

Example: STAT:OPER:CAL:ENAB?

STAT:OPER:CAL:ENAB 6	Enable bit 1 and bit 2, which allows reporting of calibration operation events to the operation status.
STAT:OPER:CAL:ENAB #B0110	The meaning is the same as above, using binary numbers.
STAT:OPER:CAL:ENAB #H06	The meaning is the same as above, using hexadecimal numbers.

:STATus:OPERation:CALibrating[:SUMMary][:EVENt]?

Function: Query the calibration operation event register. After the query, 87235 automatically clears the register.

Query: :STATus:OPERation:CALibrating[:SUMMary][:EVENt]?

Setting: Not supported

Example: STAT:OPER:CAL?

:STATus:OPERation:CALibrating[:SUMMary]:NTRansition

Function: Query or set the negative transition filter for calibration operation.

Query: :STATus:OPERation:CALibrating[:SUMMary]:NTRansition?

Setting: :STATus:OPERation:CALibrating[:SUMMary]:NTRansition <NRf>|<non-decimal number>

The parameter range is from 0 to 32767.

Example: STAT:OPER:CAL:NTR?

STAT:OPER:CAL:NTR	6	Negative transition filters the status of bit 1 and bit 2 into the event register.
STAT:OPER:CAL:NTR	#B0110	The meaning is the same as above, using binary numbers.
STAT:OPER:CAL:NTR	#H06	The meaning is the same as above, using hexadecimal numbers.

:STATus:OPERation:CALibrating[:SUMMary]:PTRansition

Function: Query or set the positive transition filter for calibration operation.

Query: :STATus:OPERation:CALibrating[:SUMMary]:PTRansition?

Setting: :STATus:OPERation:CALibrating[:SUMMary]:PTRansition <NRf>|<non-decimal number>

The parameter range is from 0 to 32767.

Example: STAT:OPER:CAL:PTR?

STAT:OPER:CAL:PTR	6	Positive transition filters the status of bit 1 and bit 2 into the event register.
STAT:OPER:CAL:PTR	#B0110	The meaning is the same as above, using binary numbers.
STAT:OPER:CAL:PTR	#H06	The meaning is the same as above, using hexadecimal numbers.

:STATus:OPERation:CONDition?

Function: Query the value in the operation status condition register.

In the return value, if bit 0 is non-zero, a calibration event is detected; if bit 5 is non-zero, a wait-for-trigger event is detected; if bit 10 is non-zero, an access to or removal event from 87235 is detected; if bit 11 is non-zero, a lower limit detection event is detected; if bit 12 is non-zero, an upper limit detection event is detected.

For example, if a calibration event is detected by this set of registers, the corresponding bits of the calibration operation enable registers (STAT:OPER:CAL:ENAB) need to be set to non-zero. Others are the same.

Query: :STATus:OPERation:CONDition?

Setting: Not supported

Example: STAT:OPER:COND?

:STATus:OPERation:ENABle

Function: Query or set the operation status event enable register. Operate by bit. 0 means that reporting status events to bit 7 (Bit7) of the status word is disabled. 1 indicates enable.

Query: :STATus:OPERation:ENABle?

Setting: :STATus:OPERation:ENABle <NRf>|<non-decimal number>
The parameter range is from 0 to 32767.

Example: STAT:OPER:ENAB?

STAT:OPER:ENAB 1	Enable bit 1, which allows reporting of operation events into the status word.
STAT:OPER:ENAB #B0001	The meaning is the same as above, using binary numbers.
STAT:OPER:ENAB #H01	The meaning is the same as above, using hexadecimal numbers.

:STATus:OPERation[:EVENt]?

Function: Query the operation status event register. After the query, 87235 automatically clears the register.

Query: :STATus:OPERation[:EVENt]?

Setting: Not supported

Example: STAT:OPER?

:STATus:OPERation:NTRansition

Function: Query or set the negative transition filter for operation state.

Query: :STATus:OPERation:NTRansition?

Setting: :STATus:OPERation:NTRansition <NRf>|<non-decimal number>
The parameter range is from 0 to 32767.

Example: STAT:OPER:NTR?

STAT:OPER:NTR 1	Negative transition filters the status of bit 0 into the event register.
STAT:OPER:NTR #B0001	The meaning is the same as above, using binary numbers.
STAT:OPER:NTR #H01	The meaning is the same as above, using hexadecimal numbers.

:STATus:OPERation:PTRansition

Function: Query or set the positive transition filter for operation state.

Query: :STATus:OPERation:NTRansition?

Setting: :STATus:OPERation:NTRansition <NRf>|<non-decimal number>

The parameter range is from 0 to 32767.

Example: STAT:OPER:NTR?

STAT:OPER:NTR #H06	Positive transition filters the status of bit 1 and bit 2 into the event register.
STAT:OPER:NTR #B0110	The meaning is the same as above, using binary numbers.
STAT:OPER:NTR 6	The meaning is the same as above, using decimal numbers.

:STATus:OPERation:LLFail[:SUMMary]:CONDition?

Function: Query the value in the lower limit detection operation status condition register.

In the return value, if bit 3 is non-zero, it indicates that the lower limit detection operation failure status of Measurement 1; if bit 4 is non-zero, it indicates that the lower limit detection operation failure status of Measurement 2; if bit 5 is non-zero, it indicates that the lower limit detection operation failure status of Measurement 3; if bit 6 is non-zero, it indicates that the lower limit detection operation failure status of Measurement 4.

Query: :STATus:OPERation:LLFail[:SUMMary]:CONDition?

Setting: Not supported

Example: STAT:OPER:LLF:COND?

:STATus:OPERation:LLFail[:SUMMary]:ENABle

Function: Query or set the event enable register for lower limit detection operation. Operate by bit. 0 means that reporting of status events to bit 11 (Bit11) of the operation status is disabled. 1 indicates enable.

Query: :STATus:OPERation:LLFail[:SUMMary]:ENABle?

Setting: :STATus:OPERation:LLFail[:SUMMary]:ENABle <NRf>|<non-decimal number>

The parameter range is from 0 to 32767.

Example: STAT:OPER:LLF:ENAB?

STAT:OPER:LLF:ENAB 8	Enable bit 3, which allows reporting of lower limit operation events to the operation status.
STAT:OPER:LLF:ENAB #B1000	The meaning is the same as above, using binary numbers.
STAT:OPER:LLF:ENAB #H08	The meaning is the same as above, using hexadecimal numbers.

:STATus:OPERation:LLFail[:SUMMary][:EVENt]?

Function: Query the event register for lower limit detection operation. After the query, 87235 automatically clears the register.

Query: :STATus:OPERation:LLFail[:SUMMary][:EVENt]?

Setting: Not supported

Example: STAT:OPER:LLF?

:STATus:OPERation:LLFail[:SUMMary]:NTRansition

Function: Query or set the negative transition filter for lower limit detection operation.

Query: :STATus:OPERation:LLFail[:SUMMary]:NTRansition?

Setting: :STATus:OPERation:LLFail[:SUMMary]:NTRansition <NRf>|<non-decimal number>

The parameter range is from 0 to 32767.

Example: STAT:OPER:LLF:NTR?

STAT:OPER:LLF:NTR	8	Negative transition filters the status of bit 3 into the event register.
STAT:OPER:LLF:NTR	#B1000	The meaning is the same as above, using binary numbers.
STAT:OPER:LLF:NTR	#H08	The meaning is the same as above, using hexadecimal numbers.

:STATus:OPERation:LLFail[:SUMMary]:PTRansition

Function: Query or set the positive transition filter for lower limit detection operation.

Query: :STATus:OPERation:LLFail[:SUMMary]:PTRansition?

Setting: :STATus:OPERation:LLFail[:SUMMary]:PTRansition <NRf>|<non-decimal number>

The parameter range is from 0 to 32767.

Example: STAT:OPER:LLF:PTR?

STAT:OPER:LLF:PTR	8	Positive transition filters the status of bit 3 into the event register.
STAT:OPER:LLF:PTR	#B1000	The meaning is the same as above, using binary numbers.
STAT:OPER:LLF:PTR	#H08	The meaning is the same as above, using decimal numbers.

:STATus:OPERation:SENSe[:SUMMary]:CONDition?

Function: Query the value in the sensor operation status condition register.

In the return value, if bit 1 is non-zero, it indicates that Channel A reads EEPROM status; If bit 2 is non-zero, it indicates that Channel B reads EEPROM status.

Query: :STATus:OPERation:SENSe[:SUMMary]:CONDition?

Setting: Not supported

Example: STAT:OPER:SENS:COND?

:STATus:OPERation:SENSe[:SUMMary]:ENABle

Function: Query or set the sensor operation event enable register. Operate by bit. 0 indicates that the sensing operation status event is disabled into bit 10 (Bit10) of the operation status. 1 indicates enable.

Query: :STATus:OPERation:SENSe[:SUMMary]:ENABle?

Setting: :STATus:OPERation:SENSe[:SUMMary]:ENABle <NRf>|<non-decimal

number>

The parameter range is from 0 to 32767.

Example: STAT:OPER:SENS:ENAB?

STAT:OPER:SENS:ENAB 6	Enable bit 1 and bit 2, which allows reporting of sensing operation events to the operation status.
STAT:OPER:SENS:ENAB #B0110	The meaning is the same as above, using binary numbers.
STAT:OPER:SENS:ENAB #H06	The meaning is the same as above, using hexadecimal numbers.

:STATus:OPERation:SENSe[:SUMMary][:EVENt]?

Function: Query the sensing operation event register. After the query, 87235 automatically clears the register.

Query: :STATus:OPERation:SENSe[:SUMMary][:EVENt]?

Setting: Not supported

Example: STAT:OPER:SENS?

:STATus:OPERation:SENSe[:SUMMary]:NTRansition

Function: Query or set the negative transition filter for sensing operation.

Query: :STATus:OPERation:SENSe[:SUMMary]:NTRansition?

Setting: :STATus:OPERation:SENSe[:SUMMary]:NTRansition <NRf>|<non-decimal number>

The parameter range is from 0 to 32767.

Example: STAT:OPER:SENS:NTR?

STAT:OPER:SENS:NTR 6	Negative transition filters the status of bit 1 and bit 2 into the event register.
STAT:OPER:SENS:NTR #B0110	The meaning is the same as above, using binary numbers.
STAT:OPER:SENS:NTR #H06	The meaning is the same as above, using hexadecimal numbers.

:STATus:OPERation:SENSe[:SUMMary]:PTRansition

Function: Query or set the positive transition filter for sensing operation.

Query: :STATus:OPERation:SENSe[:SUMMary]:PTRansition?

Setting: :STATus:OPERation:SENSe[:SUMMary]:PTRansition <NRf>|<non-decimal number>

The parameter range is from 0 to 32767.

Example: STAT:OPER:SENS:PTR?

STAT:OPER:SENS:PTR 6	Positive transition filters the status of bit 1 and bit 2 into the event register.
STAT:OPER:SENS:PTR #B0110	The meaning is the same as above, using binary numbers.

STAT:OPER:SENS:PTR #H06	The meaning is the same as above, using hexadecimal numbers.

:STATus:OPERation:TRIGger[:SUMMary]:CONDition?

Function: Query the value in the trigger operation status condition register.

In the return value, if bit 1 is non-zero, it indicates that Channel A is in Wait for Trigger; If bit 2 is non-zero, it indicates that Channel B is in Wait for Trigger. For example, returning 2 indicates that Channel A is in Wait for Trigger.

Query: :STATus:OPERation:CALibrating[:SUMMary]:CONDition?

Setting: Not supported

Example: STAT:OPER:CAL:COND?

:STATus:OPERation:TRIGger[:SUMMary]:ENABle

Function: Query or set the trigger operation event enable register. Operate by bit. 0 means that reporting of status events to bit 5 (Bit5) of the operation status is disabled. 1 indicates enable.

Query: :STATus:OPERation:TRIGger[:SUMMary]:ENABle?

Setting: :STATus:OPERation:TRIGger[:SUMMary]:ENABle <NRf>|<non-decimal number>

The parameter range is from 0 to 32767.

Example: STAT:OPER:TRIG:ENAB?

STAT:OPER:TRIG:ENAB 6	Enable bit 1 and bit 2, which allows reporting of trigger operation events to the operation status.
STAT:OPER:TRIG:ENAB #B0110	The meaning is the same as above, using binary numbers.
STAT:OPER:TRIG:ENAB #H06	The meaning is the same as above, using hexadecimal numbers.

:STATus:OPERation:TRIGger[:SUMMary][:EVENt]?

Function: Query the trigger operation event register. After the query, 87235 automatically clears the register.

Query: :STATus:OPERation:TRIGger[:SUMMary][:EVENt]?

Setting: Not supported

Example: STAT:OPER:TRIG?

:STATus:OPERation:TRIGger[:SUMMary]:NTRansition

Function: Query or set the negative transition filter for trigger operation.

Query: :STATus:OPERation:TRIGger[:SUMMary]:NTRansition?

Setting: :STATus:OPERation:TRIGger[:SUMMary]:NTRansition <NRf>|<non-decimal number>

The parameter range is from 0 to 32767.

Example: STAT:OPER:TRIG:NTR?

STAT:OPER:TRIG:NTR	6	Negative transition filters the status of bit 1 and bit 2 into the event register.
STAT:OPER:TRIG:NTR	#B0110	The meaning is the same as above, using binary numbers.
STAT:OPER:TRIG:NTR	#H06	The meaning is the same as above, using hexadecimal numbers.

:STATus:OPERation:TRIGger[:SUMMary]:PTRansition

Function: Query or set the positive transition filter for trigger operation.

Query: :STATus:OPERation:TRIGger[:SUMMary]:PTRansition?

Setting: :STATus:OPERation:TRIGger[:SUMMary]:PTRansition <NRf>|<non-decimal number>

The parameter range is from 0 to 32767.

Example: STAT:OPER:TRIG:PTR?

STAT:OPER:TRIG:PTR	6	Positive transition filters the status of bit 1 and bit 2 into the event register.
STAT:OPER:TRIG:PTR	#B0110	The meaning is the same as above, using binary numbers.
STAT:OPER:TRIG:PTR	#H06	The meaning is the same as above, using hexadecimal numbers.

:STATus:OPERation:ULFail[:SUMMary]:CONDition?

Function: Query the value in the upper limit detection operation status condition register.

In the return value, if bit 3 is non-zero, it indicates that the upper limit detection operation failure status of Measurement 1; if bit 4 is non-zero, it indicates that the upper limit detection operation failure status of Measurement 2; if bit 5 is non-zero, it indicates that the upper limit detection operation failure status of Measurement 3; if bit 6 is non-zero, it indicates that the upper limit detection operation failure status of Measurement 4.

Query: :STATus:OPERation:ULFail[:SUMMary]:CONDition?

Setting: Not supported

Example: STAT:OPER:ULF:COND?

:STATus:OPERation:ULFail[:SUMMary]:ENABle

Function: Query or set the event enable register for upper limit detection operation. Operate by bit. 0 means that reporting of status events to bit 12 (Bit12) of the operation status is disabled. 1 indicates enable.

Query: :STATus:OPERation:ULFail[:SUMMary]:ENABle?

Setting: :STATus:OPERation:ULFail[:SUMMary]:ENABle <NRf>|<non-decimal number>

The parameter range is from 0 to 32767.

Example:

STAT:OPER:ULF:ENAB?		Query the value of the upper limit detection operation event enable register.
STAT:OPER:ULF:ENAB	8	Enable bit 3, which allows reporting of

upper limit operation events to the operation status.

STAT:OPER:ULF:ENAB	#B1000	The meaning is the same as above, using binary numbers.
STAT:OPER:ULF:ENAB	#H08	The meaning is the same as above, using hexadecimal numbers.

:STATus:OPERation:ULFail[:SUMMary][:EVENt]?

Function: Query the event register for upper limit detection operation. After the query, 87235 automatically clears the register.

Query: :STATus:OPERation:ULFail[:SUMMary][:EVENt]?

Setting: Not supported

Example: STAT:OPER:ULF?

:STATus:OPERation:ULFail[:SUMMary]:NTRansition

Function: Query or set the negative transition filter for upper limit detection operation.

Query: :STATus:OPERation:ULFail[:SUMMary]:NTRansition?

Setting: :STATus:OPERation:ULFail[:SUMMary]:NTRansition <NRf>|<non-decimal number>

The parameter range is from 0 to 32767.

Example: STAT:OPER:ULF:NTR?

STAT:OPER:ULF:NTR	8	Negative transition filters the status of bit 3 into the event register.
STAT:OPER:ULF:NTR	#B1000	The meaning is the same as above, using binary numbers.
STAT:OPER:ULF:NTR	#H08	The meaning is the same as above, using hexadecimal numbers.

:STATus:OPERation:ULFail[:SUMMary]:PTRansition

Function: Query or set the positive transition filter for upper limit detection operation.

Query: :STATus:OPERation:ULFail[:SUMMary]:PTRansition?

Setting: :STATus:OPERation:ULFail[:SUMMary]:PTRansition <NRf>|<non-decimal number>

The parameter range is from 0 to 32767.

Example: STAT:OPER:ULF:PTR?

STAT:OPER:ULF:PTR	8	Positive transition filters the status of bit 1 and bit 2 into the event register.
STAT:OPER:ULF:PTR	#B1000	The meaning is the same as above, using binary numbers.
STAT:OPER:ULF:PTR	#H08	The meaning is the same as above, using decimal numbers.

:STATus:PRESet

Function: Preset some status registers as follows, and other registers remain unchanged.

Query: Not supported

Setting: :STATus:PRESet

Example: STAT:PRES

Table 3.21 Operation status register description

Register	Sub register	Preset status
OPERation	ENABle	All 0
	PTR	All 1
	NTR	All 0
QUEStionable	ENABle	All 0
	PTR	All 1
	NTR	All 0
Other	ENABle	All 0
	PTR	All 1
	NTR	All 0

:STATus:QUEStionable:CALibration[:SUMMary]:CONDition?

Function: Query the value in the calibration question status condition register.

In the return value, if bit 1 is non-zero, it indicates that Channel A is zeroed and calibrated incorrectly; if bit 2 is non-zero, it indicates that Channel B is zeroed or calibrated incorrectly. For example, returning 2 indicates that Channel A is zeroed or calibrated incorrectly.

Query: :STATus:OPERation:CALibrating[:SUMMary]:CONDition?

Setting: Not supported

Example: STAT:OPER:CAL:COND?

:STATus:QUEStionable:CALibration[:SUMMary]:ENABle

Function: Query or set the calibration question event enable register. Operate by bit. 0 indicates that reporting status events to bit 8 (Bit8) of the question status is disabled. 1 indicates enable.

Query: :STATus:QUEStionable:CALibration[:SUMMary]:ENABle?

Setting: :STATus:QUEStionable:CALibration[:SUMMary]:ENABle <NRf>|<non-decimal number>

The parameter range is from 0 to 32767.

Example: STAT:QUES:CAL:ENAB?

STAT:QUES:CAL:ENAB 6 Enable bit 1 and bit 2, which allows reporting of calibration question events

to the question status.

STAT:QUES:CAL:ENAB #B0110	The meaning is the same as above, using binary numbers.
STAT:QUES:CAL:ENAB #H06	The meaning is the same as above, using hexadecimal numbers.

:STATus:QUEStionable:CALibration[:SUMMary][:EVENt]?

Function: Query the calibration question event register. After the query, 87235 automatically clears the register.

Query: :STATus:QUEStionable:CALibration[:SUMMary][:EVENt]?

Setting: Not supported

Example: STAT:QUES:CAL?

:STATus:QUEStionable:CALibration[:SUMMary]:NTRansition

Function: Query or set the negative transition filter for calibration question.

Query: :STATus:QUEStionable:CALibration[:SUMMary]:NTRansition?

Setting: :STATus:QUEStionable:CALibration[:SUMMary]:NTRansition <NRf>|<non-decimal number>

The parameter range is from 0 to 32767.

Example: STAT:QUES:CAL:NTR?

STAT:QUES:CAL:NTR 6	Negative transition filters the status of bit 1 and bit 2 into the event register.
STAT:QUES:CAL:NTR #B0110	The meaning is the same as above, using binary numbers.
STAT:QUES:CAL:NTR #H06	The meaning is the same as above, using hexadecimal numbers.

:STATus:QUEStionable:CALibration[:SUMMary]:PTRansition

Function: Query or set the positive transition filter for calibration question.

Query: :STATus:QUEStionable:CALibration[:SUMMary]:PTRansition?

Setting: :STATus:QUEStionable:CALibration[:SUMMary]:PTRansition <NRf>|<non-decimal number>

The parameter range is from 0 to 32767.

Example: STAT:QUES:CAL:PTR?

STAT:QUES:CAL:PTR 6	Positive transition filters the status of bit 1 and bit 2 into the event register.
STAT:QUES:CAL:PTR #B0110	The meaning is the same as above, using binary numbers.
STAT:QUES:CAL:PTR #H06	The meaning is the same as above, using hexadecimal numbers.

:STATus:QUEStionable:CONDition?

Function: Query the value in the question status condition register.

In the return value, if bit 3 is non-zero, it indicates that a power question event is detected; if bit 8 is non-zero, it indicates that a calibration question event is detected; if bit 9 is non-zero, it indicates that the power-on self-test failed.

For example, if a calibration question event is detected by this set of registers, the corresponding bit of the calibration question enable register (STAT:QUES:CAL:ENAB) needs to be set non-zero. Others are the same.

Query: :STATus:QUEStionable:CONDition?

Setting: Not supported

Example: STAT:QUES:COND?

:STATus:QUEStionable:ENABle

Function: Query or set the question status event enable register. Operate by bit. 0 means that reporting status events to bit 3 (Bit3) of the status word is disabled. 1 indicates enable.

Query: :STATus:QUEStionable:ENABle?

Setting: :STATus:QUEStionable:ENABle <NRf>|<non-decimal number>

The parameter range is from 0 to 32767.

Example: STAT:QUES:ENAB?

STAT:QUES:ENAB 8	Enable bit 1, which allows reporting of calibration question events into the status word.
STAT:QUES:ENAB #B1000	The meaning is the same as above, using binary numbers.
STAT:QUES:ENAB #H08	The meaning is the same as above, using hexadecimal numbers.

:STATus:QUEStionable[:EVENt]?

Function: Query the question status event register. After the query, 87235 automatically clears the register.

Query: :STATus:QUEStionable[:EVENt]?

Setting: Not supported

Example: STAT:QUES?

:STATus:QUEStionable:NTRansition

Function: Query or set the negative transition filter for question status.

Query: :STATus:QUEStionable:NTRansition?

Setting: :STATus:QUEStionable:NTRansition <NRf>|<non-decimal number>

The parameter range is from 0 to 32767.

Example: STAT:QUES:NTR?

STAT:QUES:NTR 8	Negative transition filters the status of bit 3 into the event register.
STAT:QUES:NTR #B1000	The meaning is the same as above, using binary numbers.

STAT:QUES:NTR #H08	The meaning is the same as above, using hexadecimal numbers.

:STATus:QUEStionable:PTRansition

Function: Query or set the positive transition filter for question status.

Query: :STATus:QUEStionable:PTRansition?

Setting: :STATus:QUEStionable:PTRansition <NRf>|<non-decimal number>

The parameter range is from 0 to 32767.

Example: STAT:QUES:PTR?

STAT:QUES:PTR 8	Positive transition filters the status of bit 3 into the event register.
STAT:QUES:PTR #B0110	The meaning is the same as above, using binary numbers.
STAT:QUES:PTR #H08	The meaning is the same as above, using hexadecimal numbers.

:STATus:QUEStionable:POWer[:SUMMary]:CONDition?

Function: Query the value in the power question status condition register.

In the return value,

If bit 1 is non-zero, it indicates that the Channel A input is overloaded;

If bit 2 is non-zero, it indicates that the Channel B input is overloaded;

If bit 3 is non-zero, it indicates that the Channel A needs to be zeroed;

If bit 4 is non-zero, it indicates that the Channel B needs to be zeroed;

If bit 5 is non-zero, it indicates that the Measurement 1 data is invalid, or logarithmically incorrect;

If bit 6 is non-zero, it indicates that the Measurement 2 data is invalid, or logarithmically incorrect;

If bit 7 is non-zero, it indicates that the Measurement 3 data is invalid, or logarithmically incorrect;

If bit 8 is non-zero, it indicates that the measurement 4 data is invalid, or logarithmically incorrect.

If, for example, 8 is returned, it indicates that Channel A needs to be zeroed.

Query: :STATus:QUEStionable:POWer[:SUMMary]:CONDition?

Setting: Not supported

Example: STAT:QUES:POW:COND?

:STATus:QUEStionable:POWer[:SUMMary]:ENABle

Function: Query or set the power question event enable register. Operate by bit. 0 indicates that reporting status events to bit 3 (Bit3) of the question status is disabled. 1 indicates enable.

Query: :STATus:QUEStionable:POWer[:SUMMary]:ENABle?

Setting: :STATus:QUEStionable:POWer[:SUMMary]:ENABle <NRf>|<non-decimal number>

The parameter range is from 0 to 32767.

Example: STAT:QUES:POW:ENAB?

STAT:QUES:POW:ENAB 6	Enable bit 1 and bit 2, which allows reporting of power question events to the question status.
STAT:QUES:POW:ENAB #B0110	The meaning is the same as above, using binary numbers.
STAT:QUES:POW:ENAB #H06	The meaning is the same as above, using hexadecimal numbers.

:STATus:QUEStionable:POWer[:SUMMary][:EVENt]?

Function: Query the power question event register. After the query, 87235 automatically clears the register.

Query: :STATus:QUEStionable:POWer[:SUMMary][:EVENt]?

Setting: Not supported

Example: STAT:QUES:POW?

:STATus:QUEStionable:POWer[:SUMMary]:NTRansition

Function: Query or set the negative transition filter for power question.

Query: :STATus:QUEStionable:POWer[:SUMMary]:NTRansition?

Setting: :STATus:QUEStionable:POWer[:SUMMary]:NTRansition <NRf>|< non decimal number >

The parameter range is from 0 to 32767.

Example: STAT:QUES:POW:NTR?

STAT:QUES:POW:NTR 6	Negative transition filters the status of bit 1 and bit 2 into the event register.
STAT:QUES:POW:NTR #B0110	The meaning is the same as above, using binary numbers.
STAT:QUES:POW:NTR #H06	The meaning is the same as above, using hexadecimal numbers.

:STATus:QUEStionable:POWer[:SUMMary]:PTRansition

Function: Query or set the positive transition filter for power question.

Query: :STATus:QUEStionable:POWer[:SUMMary]:PTRansition?


Setting: :STATus:QUEStionable:POWer[:SUMMary]:PTRansition <NRf>|< non decimal number >

The parameter range is from 0 to 32767.

Example: STAT:QUES:POW:PTR?

STAT:QUES:POW:PTR 6	Positive transition filters the status of bit 1 and bit 2 into the event register.
STAT:QUES:POW:PTR #B0110	The meaning is the same as above, using binary numbers.
STAT:QUES:POW:PTR #H06	The meaning is the same as above, using hexadecimal numbers.

Attachment: Status Block Diagram

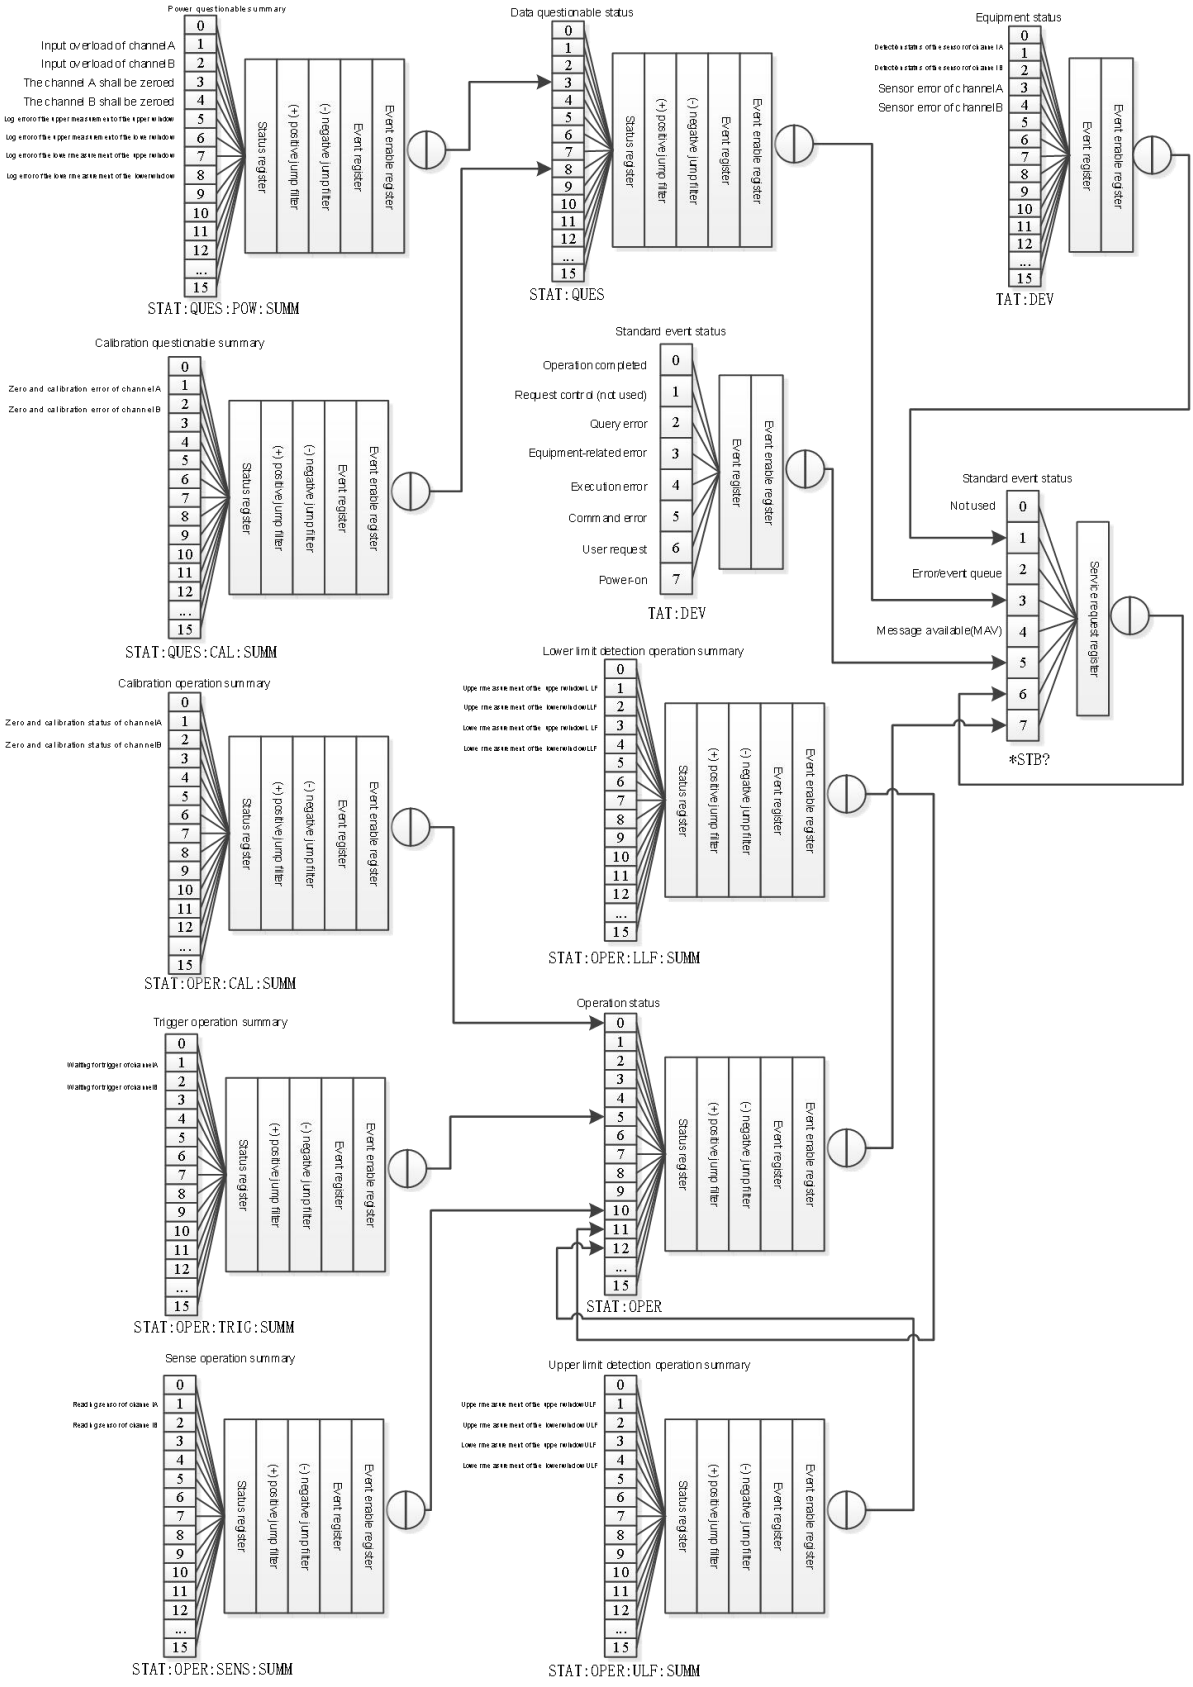

3.3.9 System Subsystem Command (SYSTem)

- :SYSTem:ERRor:CODE?.....128
- :SYSTem:ERRor[:NEXT]?.....128
- :SYSTem:HELP:HEADers?.....128
- :SYSTem:IDN.....129
- :SYSTem:IDN:AUTO.....129
- :SYSTem:PRESet.....129
- :SYSTem:VERSion?.....142

:SYSTem:ERRor:CODE?

Function: Return the error code from the error queue of the 87235. When an error is generated, the error code is stored in the error queue. Every time this command is executed, this message will be removed from the error queue. The order of error messages out of the queue is first-in-first-out (FIFO), i.e., the oldest messages go out of the queue first. The error queue can be cleared with the *CLS command. Executing this command when the error queue is empty will return 0. The error queue can hold up to 1000 error messages.

Query: :SYSTem:ERRor:CODE?

Setting: Not supported

Example: SYST:ERR:CODE? Query error code

Reset state: None.

:SYSTem:ERRor[:NEXT]?

Function: Return the error code and error message from the error queue of the 87235. When an error is generated, the error code and error message are stored in the error queue. Every time this command is executed, this message will be removed from the error queue. The order of error messages out of the queue is first-in-first-out (FIFO), i.e., the oldest messages go out of the queue first. The error queue can be cleared with the *CLS command. Executing this command when the error queue is empty will return "0, "No Error"". The error queue can hold up to 1000 error messages.

Query: :SYSTem:ERRor[:NEXT]?

Setting: Not supported

Example: SYST:ERR?

Reset state: None.

:SYSTem:HELP:HEADers?

Function: Query the list of commands supported by 87235. The data format is <Arbitrary data block>. See Section 7.7.6 of IEEE 488.2.

#nNNN...Nddd……ddd<LF>

Data newline character indicating the end of the data block.
Data length (i.e., the number of bytes of d)
Number of bits of data length (i.e., the number of bits of N)
The marker for the start of the data block.

The data block is of the form #510331 ..... in <LF> n = 5 and N = 10331.

Query: :SYSTem:HELP:HEADers?

Setting: Not supported

Example: SYST:HELP:HEAD?

Reset state: None.

:SYSTem:IDN

Function: Query or set the user-defined string of the 87235.
Related program control commands ":SYSTem:IDN:AUTO", "*IDN?"

Query: :SYSTem:IDN?

Setting: :SYSTem:IDN <string parameters>
Valid forms of string parameters are "A, B, C, D"
Where A stands for the name of the manufacturer, such as Ceyear
B stands for the product model, such as 87235D
C stands for product serial number, such as SN01
D stands for the version number of the product, such as 1.0.0

Example:

SYST:IDN?	Return the current user-defined IDN return string.
SYST:IDN "Ceyear,87235D,001,1.0"	Set the user-defined IDN return string

Reset state: None.

:SYSTem:IDN:AUTO

Function: Enable or disable user-defined strings,
ON: Allows users to query and set user-defined strings via ":SYSTem:IDN", "*IDN?".
OFF: Disable users to query and set user-defined strings via ":SYSTem:IDN" and "*IDN?".
Related program control commands ":SYSTem:IDN", "*IDN?"

Query: :SYSTem:IDN:AUTO?

Setting: :SYSTem:IDN:AUTO <Boolean data>
Valid forms of <Boolean data> are: 0, OFF, 1, ON

Example:

SYST:IDN:AUTO?	Query the switch state of user-defined.
SYST:IDN:AUTO 1	Enable user-defined strings.
SYST:IDN:AUTO 0	Disable user-defined strings.

Reset state: Off

:SYSTem:PRESet

Function: Reset 87235 to the state specified by the parameter. A total of 23 states are offered in this case.

Query: Not supported

Setting: :SYSTem:PRESet [character data]

The form of [character data] is as follows (DEFault is the default parameter, i.e., the parameter when no parameters are included.) :

- DEFault.....130
- GSM900.....132
- EDGE.....133
- CDMAone.....133
- CDMA2000.....134
- WCDMA.....134
- BLUetooth.....134
- MCPa.....135
- RADar.....136
- WL802DOT11A.....136
- HIPERLAN2.....136
- WL802DOT11B.....137
- XEVDO.....137
- XEVDV.....137
- TDSCdma.....137
- NADC.....138
- IDEN.....138
- DVB.....139
- WIMAX.....139
- DME.....140
- DMEPRT.....141
- HSDPA.....141
- LTE.....141

Example: SYST:PRES GSM900 Reset state to GSM900.

Reset state: See the table below.

1) DEFault

Table 3.22 Default reset state (DEFault)

Command	Setting:	Description
CALC[1]|2|3|4:FEED[1]|2	"POW:AVER"	Set the average measurement mode
CALC[1]|2|3|4:GAIN[:MAGN]	0.000dB	Set the calculation offset to 0
CALC[1]|2|3|4:GAIN:STAT	OFF	Disable the calculation offset

CALC[1]|2|3|4:LIM:CLE:AUTO	ON	Clear the limit detection state when initializing the measurement
CALC[1]|2|3|4:LIM:LOW[:DATA]	-90dBm	Lower limit
CALC[1]|2|3|4:LIM:STAT	OFF	Disable the measurement limit detection
CALC[1]|2|3|4:LIM:UPP[:DATA]	90dBm	Upper limit
CALC[1]|2|3|4:MATH[:EXPR]	SENS1	Measurement expression
CALC[1]|2|3|4:REL[:MAGN]:AUTO	OFF	Disable the reference value of the relative measurement.
CALC[1]|2|3|4:REL:STAT	OFF	Disable relative measurement.
CAL[1]|2:RCAL	No effect	The switch must be calibrated to be unaffected.
DISP[:WIND[1]|2][:NUM[1]|2]:RES	3	Measurement display resolution is set to 3
FORM[:READ]:BORD	NORMal	The byte order of binary data is normal.
FORM[:READ][:DATA]	ASCii	The data format is ASCII
INIT[1]|2:CONT	ON	In Wait for Trigger state
MEM:TABL:SEL	No effect	Current frequency response offset table
[SENS[1]]:AVER:COUN	8	Filter length
[SENS[1]]:AVER:COUN:AUTO	ON	Turn on Auto Average.
[SENS[1]]:AVER:SDET	ON	Turn on the step detection
[SENS[1]]:AVER[:STAT]	ON	Turn on the average
[SENS[1]]:CORR:CSET2[:SEL]	No effect	Currently selected frequency response offset table
[SENS[1]]:CORR:CSET2:STAT	No effect	The switch status of the currently selected frequency response offset table
[SENS[1]]:CORR:FDOF|GAIN4[:INP][:MAGN]	No effect	Return the frequency response bias value
[SENS[1]]:CORR:GAIN2:STAT	OFF	Disable the channel

		offset
[SENS[1]]:CORR:GAIN2:[:INPut][:MAGNitude]	0.00dB	Channel offset is 0
[SENS[1]]:FREQ[:CW|:FIX]	1GHz	Channel frequency is 1GHz
[SENS[1]]:SWE[1]|2|3|4:OFFS:TIME	0	Set the start time of gate
[SENS[1]]:SWE[1]|2|3|4:TIME	Gate 1: 100us Other: 0	Set the length of gate
[SENS[1]]:TRACe:OFFSet:TIME	0	Set the minimum display time of trace
[SENS[1]]:TRACe:TIME	100us	Set the display time length of trace to 100us
TRAC[1]|2:UNIT	dBm	Trace display unit
TRACe[1]|2:DEFine:TRANsition:REFerence	10%, 90%	Pulse transition reference.
TRIG[:SEQ]:DEL	0	Trigger delay
TRIG[:SEQ]:LEV	-5 dBm	Trigger level
TRIG[:SEQ]:SLOP	POS	Rising edge trigger
TRIG[:SEQ[1]|2]:SOUR	IMM	Trigger source
UNIT:POW	dBm	Power unit
UNIT:POW:RAT	dB	Rate unit

2) GSM900

Global System for Mobile Communications, commonly known as GSM,

uses a digital modulation method called 0.3GMSK (Gaussian Minimum Shift Keying). 0.3 indicates the ratio of Gaussian filter bandwidth to bit rate. GMSK is a special type of digital FM modulation. Adding or subtracting 67.708 KHz to the RF carrier frequency indicates 1 and 0. The modulation technique that uses two frequencies to represent 1 and 0 is noted as FSK (frequency shift keying).

In GSM, the data rate is chosen to be 270.833 kbit/sec, exactly four times the RF frequency offset, which minimizes the modulation spectrum and improves the channel efficiency.

FSK modulation with a bit rate exactly 4 times the frequency offset is called MSK (minimum frequency shift keying). In GSM, a Gaussian pre-modulation filter is used to further reduce the modulation spectrum. It reduces the speed of frequency conversion, which would otherwise result in radiated energy to adjacent channels. The parts of the following settings that are not enumerated are the same as DEFault.

Table 3.23 GSM900 preset status

Command	Setting:	Description
[SENS[1]]:FREQ[:CW|:FIX]	900MHz	Channel frequency
[SENS[1]]:SWE[1]|2|3|4:OFFS:TIME	Gate 1: 20us	Set the start time of gate

	Other: 0	
[SENS[1]]:SWE[1]|2|3|4:TIME	Gate 1: 520us Other: 0	Set the length of gate
[SENS[1]]:TRACe:OFFSet:TIME	0	Set the minimum display time of trace
[SENS[1]]:TRACe:TIME	1ms	Set the display time length of trace to 1ms
TRIG[:SEQ]:DEL	-20 μs	Trigger delay
TRIG[:SEQ]:LEV	-5 dBm	Trigger level
TRIG[:SEQ]:SLOP	POS	Rising edge trigger
TRIG[:SEQ[1]|2]:SOUR	INT1	Trigger source

3) EDGE

Enhanced Data for Global Evolution or Enhanced Data for GSM Evolution.

EDGE is a transition technology from GSM to 3G, which mainly uses a new modulation method in GSM systems, namely the state-of-the-art multi-time slot operation and 8PSK modulation technology. Since 8PSK can extend the signal space of the GMSK modulation technique used in existing GSM networks from 2 to 8, this allows each symbol to contain four times more information.

The parts of the following settings that are not enumerated are the same as DEFault.

Table 3.24 EDGE preset status

Command	Setting:	Description
[SENS[1]]:FREQ[:CW|:FIX]	900MHz	Channel frequency
[SENS[1]]:SWE[1]|2|3|4:OFFS:TIME	Gate 1: 20us Other: 0	Set the start time of gate
[SENS[1]]:SWE[1]|2|3|4:TIME	Gate 1: 520us Other: 0	Set the length of gate
[SENS[1]]:TRACe:OFFSet:TIME	0	Set the minimum display time of trace
[SENS[1]]:TRACe:TIME	1ms	Set the display time length of trace to 1ms
TRIG[:SEQ]:DEL	-40 μs	Trigger delay
TRIG[:SEQ]:LEV	-5 dBm	Trigger level
TRIG[:SEQ]:SLOP	POS	Rising edge trigger
TRIG[:SEQ[1]|2]:SOUR	INT1	Trigger source

4) CDMAone

CDMAone is a 2G mobile communication standard. The underlying signaling standard is IS-95, a 2G mobile standard developed by Qualcomm and TIA based on CDMA technology. CDG applied for the trademark cdmaOne for this technology, and cdmaOne and its associated standards were the first commercially available mobile communications standards based on CDMA technology.

3.3 Instrument Subsystem Command

IS-95 is the number assigned by TIA to the most prominent air interface standard for 2G mobile communications based on CDMA technology, known as Interim Standard 95.

The parts of the following settings that are not enumerated are the same as DEFault.

Table 3.25 CDMAone preset status

Command	Setting:	Description
[SENS[1]]:FREQ[:CW|:FIX]	850MHz	Channel frequency
[SENS[1]]:SWE[1]|2|3|4:OFFS:TIME	0	Set the start time of gate
[SENS[1]]:SWE[1]|2|3|4:TIME	Gate 1: 10ms Other: 0	Set the length of gate
[SENS[1]]:TRACe:OFFSet:TIME	0	Set the minimum display time of trace
[SENS[1]]:TRACe:TIME	10ms	Set the display time length of trace
TRIG[:SEQ]:DEL	0	Trigger delay
TRIG[:SEQ]:LEV	-5 dBm	Trigger level
TRIG[:SEQ]:SLOP	POS	Rising edge trigger
TRIG[:SEQ[1]|2]:SOUR	INT1	Trigger source

5) CDMA2000 and WCDMA

It is the well-known 3G 1X or 1xRTT, which is the core of 3G CDMA2000 technology. The mark 1x customarily refers to CDMA2000 wireless technology that uses a pair of 1.25 MHz radio channels.

The parts of the following settings that are not enumerated are the same as DEFault.

Table 3.26 CDMA2000 and WCDMA: preset status

Command	Setting:	Description
[SENS[1]]:FREQ[:CW|:FIX]	1.9GHz	Channel frequency
[SENS[1]]:SWE[1]|2|3|4:OFFS:TIME	0	Set the start time of gate
[SENS[1]]:SWE[1]|2|3|4:TIME	Gate 1: 10ms Other: 0	Set the length of gate
[SENS[1]]:TRACe:OFFSet:TIME	0	Set the minimum display time of trace
[SENS[1]]:TRACe:TIME	10ms	Set the display time length of trace
TRIG[:SEQ]:DEL	0	Trigger delay
TRIG[:SEQ]:LEV	-5 dBm	Trigger level
TRIG[:SEQ]:SLOP	POS	Rising edge trigger
TRIG[:SEQ[1]|2]:SOUR	INT1	Trigger source

6) BLUetooth

The parts of the following settings that are not enumerated are the same as DEFault.

Table 3.27 BLUetooth preset status

Command	Setting:	Description
[SENS[1]]:FREQ[:CW|:FIX]	2.4GHz	Channel frequency
[SENS[1]]:SWE[1]|2|3|4:OFFS:TIME	Gate 1: 200ns Other: 0	Set the start time of gate
[SENS[1]]:SWE[1]|2|3|4:TIME	Gate 1: 366us Other: 0	Set the length of gate
[SENS[1]]:TRACe:OFFSet:TIME	0	Set the minimum display time of trace
[SENS[1]]:TRACe:TIME	500us	Set the display time length of trace
TRIG[:SEQ]:DEL	0	Trigger delay
TRIG[:SEQ]:LEV	-5 dBm	Trigger level
TRIG[:SEQ]:SLOP	POS	Rising edge trigger
TRIG[:SEQ[1]|2]:SOUR	INT1	Trigger source

7) MCPa

Multi-Carrier Power Amplifier.

The ideal software radio combines multiple carriers in the transmitting direction into a one-way signal, which is upconverted and then amplified with a type of MCPA for low-noise amplification of the wideband analog mixed signal. Because the difference between the signal and signal envelope amplitude in mixed signals is large, it is particularly sensitive to amplifier nonlinearity. The MCPA uses a forward feedback technique to suppress unwanted intermodulation carriers and obtain effective power utilization. A good selection of devices and the use of circuit CAD optimization techniques are required.

The parts of the following settings that are not enumerated are the same as DEFault.

Table 3.28 MCPa preset status

Command	Setting:	Description
[SENS[1]]:FREQ[:CW|:FIX]	1.9GHz	Channel frequency
[SENS[1]]:SWE[1]|2|3|4:OFFS:TIME	0	Set the start time of gate
[SENS[1]]:SWE[1]|2|3|4:TIME	Gate 1: 10ms Other: 0	Set the length of gate
[SENS[1]]:TRACe:OFFSet:TIME	0	Set the minimum display time of trace
[SENS[1]]:TRACe:TIME	10ms	Set the display time length of trace
TRIG[:SEQ]:DEL	0	Trigger delay
TRIG[:SEQ]:LEV	-5 dBm	Trigger level
TRIG[:SEQ]:SLOP	POS	Rising edge trigger

TRIG[:SEQ[1]|2]:SOUR	INT1	Trigger source

8) RADar

The parts of the following settings that are not enumerated are the same as DEFault.

Table 3.29 RADAR: preset status

Command	Setting:	Description
[SENS[1]]:FREQ[:CW|:FIX]	10GHz	Channel frequency
[SENS[1]]:SWE[1]|2|3|4:OFFS:TIME	Gate 3: 750ns Other: 0	Set the start time of gate
[SENS[1]]:SWE[1]|2|3|4:TIME	Gate 1: 1us Gate 2: 250ns Gate 3: 250ns Other: 0	Set the length of gate
[SENS[1]]:TRACe:OFFSet:TIME	0	Set the minimum display time of trace
[SENS[1]]:TRACe:TIME	2us	Set the display time length of trace
TRIG[:SEQ]:DEL	-252ns	Trigger delay
TRIG[:SEQ]:LEV	-5 dBm	Trigger level
TRIG[:SEQ]:SLOP	POS	Rising edge trigger
TRIG[:SEQ[1]|2]:SOUR	INT1	Trigger source

9) 802.11a (WL802DOT11A) and HIPERLAN2

The parts of the following settings that are not enumerated are the same as DEFault.

Table 3.30 802.11a and HiperLan2 preset status

Command	Setting:	Description
[SENS[1]]:FREQ[:CW|:FIX]	5.2GHz	Channel frequency
[SENS[1]]:SWE[1]|2|3|4:OFFS:TIME	0	Set the start time of gate
[SENS[1]]:SWE[1]|2|3|4:TIME	Gate 1: 25us Other: 0	Set the length of gate
[SENS[1]]:TRACe:OFFSet:TIME	0	Set the minimum display time of trace
[SENS[1]]:TRACe:TIME	50us	Set the display time length of trace
TRIG[:SEQ]:DEL	0	Trigger delay
TRIG[:SEQ]:LEV	-5 dBm	Trigger level
TRIG[:SEQ]:SLOP	POS	Rising edge trigger
TRIG[:SEQ[1]|2]:SOUR	INT1	Trigger source

10) 802.11b/g (WL802DOT11B)

The parts of the following settings that are not enumerated are the same as DEFault.

Table 3.31 802.11b/g preset status

Command	Setting:	Description
[SENS[1]]:FREQ[:CW|:FIX]	2.4GHz	Channel frequency
[SENS[1]]:SWE[1]|2|3|4:OFFS:TIME	0	Set the start time of gate
[SENS[1]]:SWE[1]|2|3|4:TIME	Gate 1: 100us Other: 0	Set the length of gate
[SENS[1]]:TRACe:OFFSet:TIME	0	Set the minimum display time of trace
[SENS[1]]:TRACe:TIME	100us	Set the display time length of trace
TRIG[:SEQ]:DEL	0	Trigger delay
TRIG[:SEQ]:LEV	-5 dBm	Trigger level
TRIG[:SEQ]:SLOP	POS	Rising edge trigger
TRIG[:SEQ[1]|2]:SOUR	INT1	Trigger source

11) 1xeV-DO (XEVDO), 1xeV-DV (XEVDV) and TDSCdma

Evolution-Data Only, CDMA2000 1xEV Phase 1 Supports downlink (forward link) data rates up to 3.1 Mbps

and uplink (reverse link) rates up to 1.8 Mbps with one radio channel transmitting high-speed data message data.

1xEV-DO is already in commercial operation. The European market is slightly ahead of the U.S. market. In the summer of 2004 Czech mobile operator Eurotel began operating the sinceCDMA2000 1xEV-DO network, and they offered uplink rates of about 1 Mbps. This service costs about 30 euros per month without traffic restrictions. To use this service, you need to spend about 300 euros to buy a Gtran GPC-6420 modem.

The parts of the following settings that are not enumerated are the same as DEFault.

Table 3.32 1xeV-DO (XEVDO), 1xeV-DV (XEVDV) and TDSCdma preset status

Command	Setting:	Description
[SENS[1]]:FREQ[:CW|:FIX]	1.9GHz	Channel frequency
[SENS[1]]:SWE[1]|2|3|4:OFFS:TIME	Gate 1: 10us Other: 0	Set the start time of gate
[SENS[1]]:SWE[1]|2|3|4:TIME	Gate 1: 810us Other: 0	Set the length of gate
[SENS[1]]:TRACe:OFFSet:TIME	0	Set the minimum display time of trace

[SENS[1]]:TRACe:TIME	1ms	Set the display time length of trace to 1ms
TRIG[:SEQ]:DEL	-40 μs	Trigger delay
TRIG[:SEQ]:LEV	-5 dBm	Trigger level
TRIG[:SEQ]:SLOP	POS	Rising edge trigger
TRIG[:SEQ[1]|2]:SOUR	INT1	Trigger source

12) NADC

NADC - North American Digital Cellular

The parts of the following settings that are not enumerated are the same as DEFault.

Table 3.33 NADC preset status

Command	Setting:	Description
[SENS[1]]:FREQ[:CW|:FIX]	800MHz	Channel frequency
[SENS[1]]:SWE[1]|2|3|4:OFFS:TIME	Gate 1: 123.5us Gate 2: 20.123ms Other: 0	Set the start time of gate
[SENS[1]]:SWE[1]|2|3|4:TIME	Gate 1/2: 6.46ms Other: 0	Set the length of gate
[SENS[1]]:TRACe:OFFSet:TIME	0	Set the minimum display time of trace
[SENS[1]]:TRACe:TIME	50ms	Set the display time length of trace to 1ms
TRIG[:SEQ]:DEL	-200 μs	Trigger delay
TRIG[:SEQ]:LEV	-5 dBm	Trigger level
TRIG[:SEQ]:SLOP	POS	Rising edge trigger
TRIG[:SEQ[1]|2]:SOUR	INT1	Trigger source

13) iDEN

The parts of the following settings that are not enumerated are the same as DEFault.

Table 3.34 iDEN preset status

Command	Setting:	Description
[SENS[1]]:AVER:COUN	64	Filter length
[SENS[1]]:FREQ[:CW|:FIX]	800MHz	Channel frequency
[SENS[1]]:SWE[1]|2|3|4:OFFS:TIME	0	Set the start time of gate
[SENS[1]]:SWE[1]|2|3|4:TIME	Gate 1: 15ms Gate 2: 90ms Gate 3: 160us	Set the length of gate

	Other: 0	
[SENS[1]]:TRACe:OFFSet:TIME	0	Set the minimum display time of trace
[SENS[1]]:TRACe:TIME	100ms	Set the display time length of trace
TRIG[:SEQ]:DEL	0	Trigger delay
TRIG[:SEQ]:LEV	-5 dBm	Trigger level
TRIG[:SEQ]:SLOP	POS	Rising edge trigger
TRIG[:SEQ[1]|2]:SOUR	INT1	Trigger source

14) DVB

The parts of the following settings that are not enumerated are the same as DEFault.

Table 3.35 DVB: preset status

Command	Setting:	Description
[SENS[1]]:AVER:COUN	8	Filter length
[SENS[1]]:FREQ[:CW|:FIX]	660MHz	Channel frequency
[SENS[1]]:SWE[1]|2|3|4:OFFS:TIME	Gate 1: 10us Other: 0	Set the start time of gate
[SENS[1]]:SWE[1]|2|3|4:TIME	Gate 1: 15ms Gate 2: 90ms Other: 0	Set the length of gate
[SENS[1]]:TRACe:OFFSet:TIME	0	Set the minimum display time of trace
[SENS[1]]:TRACe:TIME	100ms	Set the display time length of trace
TRIG[:SEQ]:DEL	0	Trigger delay
TRIG[:SEQ]:LEV	-5 dBm	Trigger level
TRIG[:SEQ]:SLOP	POS	Rising edge trigger
TRIG[:SEQ[1]|2]:SOUR	INT1	Trigger source

15) WiMAX

Worldwide Interoperability for Microwave Access.

Combining this technology with microwave devices that require licensing or are license-free will expand the broadband wireless market and improve the perception of enterprises and service providers due to lower costs.

The parts of the following settings that are not enumerated are the same as DEFault.

Table 3.36 WiMAX preset status

3.3 Instrument Subsystem Command

Command	Setting:	Description
[SENS[1]]:FREQ[:CW|:FIX]	3.5GHz	Channel frequency
[SENS[1]]:SWE[1]|2|3|4:OFFS:TIME	Gate 2: 102us Other: 0	Set the start time of gate
[SENS[1]]:SWE[1]|2|3|4:TIME	Gate 1: 102us Gate 2: 306us Other: 0	Set the length of gate
[SENS[1]]:TRACe:OFFSet:TIME	0	Set the minimum display time of trace
[SENS[1]]:TRACe:TIME	1ms	Set the display time length of trace
TRIG[:SEQ]:DEL	-200us	Trigger delay
TRIG[:SEQ]:LEV	-5 dBm	Trigger level
TRIG[:SEQ]:SLOP	POS	Rising edge trigger
TRIG[:SEQ[1]|2]:SOUR	INT1	Trigger source

16) DME

The parts of the following settings that are not enumerated are the same as DEFault.

Table 3.37 DME preset status

Command	Setting:	Description
[SENS[1]]:AVER:COUN	32	Filter length
[SENS[1]]:FREQ[:CW|:FIX]	1.1GHz	Channel frequency
[SENS[1]]:SWE[1]|2|3|4:OFFS:TIME	Gate 1: -2us Gate 2: 8us Other: 0	Set the start time of gate
[SENS[1]]:SWE[1]|2|3|4:TIME	Gate 1: 8us Gate 2: 50us Other: 0	Set the length of gate
[SENS[1]]:TRACe:OFFSet:TIME	0	Set the minimum display time of trace
[SENS[1]]:TRACe:TIME	100us	Set the display time length of trace
TRACe[1]|2:DEFine:TRANsition:REFerence	1%, 81%	Pulse transition reference.
TRIG[:SEQ]:DEL	-3us	Trigger delay
TRIG[:SEQ]:LEV	-5 dBm	Trigger level
TRIG[:SEQ]:SLOP	POS	Rising edge trigger
TRIG[:SEQ[1]|2]:SOUR	INT1	Trigger source

17) DMEPRT

The parts of the following settings that are not enumerated are the same as DEFault.

Table 3.38 DME-PRT preset status

Command	Setting:	Description
[SENS[1]]:AVER:COUN	32	Filter length
[SENS[1]]:FREQ[:CW|:FIX]	1.1GHz	Channel frequency
[SENS[1]]:SWE[1]|2|3|4:OFFS:TIME	Gate 2: 8us Other: 0	Set the start time of gate
[SENS[1]]:SWE[1]|2|3|4:TIME	Gate 1: 6us Gate 2: 50us Other: 0	Set the length of gate
[SENS[1]]:TRACe:OFFSet:TIME	0	Set the minimum display time of trace
[SENS[1]]:TRACe:TIME	100us	Set the display time length of trace
TRACe[1]|2:DEFine:TRANsition:REFerence	0.25%, 9%	Pulse transition reference.
TRIG[:SEQ]:DEL	-2us	Trigger delay
TRIG[:SEQ]:LEV	-5 dBm	Trigger level
TRIG[:SEQ]:SLOP	POS	Rising edge trigger
TRIG[:SEQ[1]|2]:SOUR	INT1	Trigger source

18) HSDPA

The parts of the following settings that are not enumerated are the same as DEFault.

Table 3.39 HSDPA preset status

Command	Setting:	Description
[SENS[1]]:AVER:COUN	64	Filter length
[SENS[1]]:FREQ[:CW|:FIX]	1.9GHz	Channel frequency
[SENS[1]]:SWE[1]|2|3|4:OFFS:TIME	0	Set the start time of gate
[SENS[1]]:SWE[1]|2|3|4:TIME	Gate 1: 10ms Other: 0	Set the length of gate
[SENS[1]]:TRACe:OFFSet:TIME	0	Set the minimum display time of trace
[SENS[1]]:TRACe:TIME	10ms	Set the display time length of trace
TRIG[:SEQ]:DEL	0	Trigger delay
TRIG[:SEQ]:LEV	-5 dBm	Trigger level
TRIG[:SEQ]:SLOP	POS	Rising edge trigger
TRIG[:SEQ[1]|2]:SOUR	INT1	Trigger source

19) LTE

The parts of the following settings that are not enumerated are the same as DEFault.

LTE: Long term evolution of general-purpose mobile communications technology. Long Term Evolution, a long-term evolution of the UMTS (Universal Mobile Telecommunications System) technology standard developed by the 3GPP (The 3rd Generation Partnership Project), was formally established and launched at the 3GPP Toronto meeting in December 2004. LTE system introduces key technologies such as OFDM (Orthogonal Frequency Division Multiplexing) and MIMO (Multi-Input&Multi-Output), which significantly increase the spectral efficiency and data transmission rate (under the condition of 64QAM, the theoretical maximum downlink transmission rate of 20M bandwidth 2XMIMO is 201Mbps, which is about 150Mbps after excluding signaling overhead. However, according to the actual networking and terminal capacity constraints, it is generally considered that the downlink peak rate is 100Mbps and the uplink is 50Mbps), and it supports a variety of bandwidth allocation: 1.4MHz, 3MHz, 5MHz, 10MHz, 15MHz, 20MHz. 10MHz, 15MHz, 20MHz, etc.

Table 3.40 LTE preset status

Command	Setting:	Description
[SENS[1]]:AVER:COUN	64	Filter length
[SENS[1]]:FREQ[:CW|:FIX]	2GHz	Channel frequency
[SENS[1]]:SWE[1]|2|3|4:OFFS:TIME	0	Set the start time of gate
[SENS[1]]:SWE[1]|2|3|4:TIME	Gate 1: 1.2ms Gate 2: 10ms Other: 0	Set the length of gate
[SENS[1]]:TRACe:OFFSet:TIME	-0.2ms	Set the minimum display time of trace
[SENS[1]]:TRACe:TIME	11ms	Set the display time length of trace
TRIG[:SEQ]:DEL	0	Trigger delay
TRIG[:SEQ]:LEV	-5 dBm	Trigger level
TRIG[:SEQ]:SLOP	POS	Rising edge trigger
TRIG[:SEQ[1]|2]:SOUR	INT1	Trigger source

:SYSTem:VERSion?

Function: Query the SCPI version number used by 87235. The return form is YYYY.X, where YYYY denotes the year and X denotes the version number. It returns 1999.0 in this case.

Query: :SYSTem:VERSion?

Setting: Not supported

Example: SYST:VERS? Query the SCPI version number

Reset state: None.

3.3.10 Trigger Subsystem Command (INITiate/ TRIGger)

- :ABORt[1]……143
- :INITiate[1]:CONTinuous……143
- :INITiate:CONTinuous:ALL……144
- :INITiate:CONTinuous:SEQuence[1]……144
- :INITiate[1][:IMMediate]……145
- :INITiate[:IMMediate]:ALL……145
- :INITiate[:IMMediate]:SEQuence[1]……145
- :INPut:TRIGger:IMPedance……145
- :OUTput:TRIGger[:STATe]……146
- :TRIGger[1][:IMMediate]……145
- :TRIGger:MODE……146
- :TRIGger[:SEQuence[1]]:COUNt……147
- :TRIGger[:SEQuence[1]]:DELay……147
- :TRIGger[:SEQuence[1]]:HOLDoff……148
- :TRIGger[:SEQuence[1]]:IMMediate……148
- :TRIGger[:SEQuence[1]]:POSition……148
- :TRIGger[:SEQuence]:SLOPe……149
- :TRIGger[:SEQuence[1]]:SOURce……149

:ABORt[1]

Function: Stop the measurement of the corresponding channel of the 87235. Restart the measurement after sending INITiate:CONTinuous ON.

Query: Not supported

Setting: ABORt[1]

Example:

ABOR	Stop measuring Channel A.
ABOR	Stop measuring

Description: 87235 does not set the trigger idle state, i.e. the trigger is always in the wait state.

:INITiate[1]:CONTinuous

Function: Query or set the trigger state of the 87235: single step and continuous

When set to single-step (OFF), wait for trigger until it is set to continuous (ON), or is received

INITiate:IMMediate。

This command is equivalent to INITiate:CONTinuous:SEQuence[1]

Query: :INITiate[1]:CONTinuous?

Setting: :INITiate[1]:CONTinuous <Boolean data>

OFF | 0 Single
ON|1 Continuous

Example:	INIT:CONT?	Query the trigger state: 0 for single step and 1 for continuous.
	INIT:CONT ON	Set Channel A to continuous trigger state.

Description: For the parameter OFF, this corresponds to stopping the measurement; for the parameter ON, this corresponds to starting the measurement.

Reset state: Set to ON

:INITiate:CONTinuous:ALL

Function: Query or set the trigger state of all channels of the 87235: single step and continuous

When set to single-step (OFF), wait for trigger until it is set to continuous (ON), or INITiate:IMMediate is received.

Query: :INITiate:CONTinuous:ALL?

Setting: :INITiate:CONTinuous:ALL <Boolean data>

OFF | 0 Single
ON|1 Continuous

Example:	INIT:CONT:ALL?	Query the trigger state of all channels. When all channels are continuously triggered, it is 1, otherwise it is 0.
	INIT:CONT:ALL ON	Set all channels to continuous trigger state.

Reset state: Set to ON

:INITiate:CONTinuous:SEQuence[1]

Function: Query or set the trigger state of the 87235: single step and continuous

When set to single-step (OFF), wait for trigger until it is set to continuous (ON), or is received

INITiate:IMMediate。

This command is equivalent to INITiate[1]:CONTinuous

Query: :INITiate:CONTinuous:SEQuence[1]?

Setting: :INITiate:CONTinuous:SEQuence[1] <Boolean data>

OFF | 0 Single
ON|1 Continuous

Example:	INIT:CONT:SEQ?	Query the trigger state: 0 for single step and 1 for continuous.
	INIT:CONT:SEQ1 ON	Set Channel A to continuous trigger state.

Reset state: Set to ON

:INITiate[1][:IMMediate]

Function: Set 87235 to Wait for Trigger state. The measurement starts when a trigger event is received.
Equivalent command INITiate:[IMMediate]:SEQuence[1]

Query: Not supported

Setting: :INITiate[1][:IMMediate]

Example: INIT — Set 87235 to Wait for Trigger state.

Reset state: None

:INITiate[:IMMediate]:ALL

Function: Set all channels of the 87235 to be in Wait for Trigger state. The measurement starts when a trigger event is received.

Query: Not supported

Setting: :INITiate[:IMMediate][:ALL]

Example: INIT:ALL — Set all channels of the 87235 to be in Wait for Trigger state.

Reset state: None

:INITiate[:IMMediate]:SEQuence[1]

Function: Set 87235 to Wait for Trigger state. The measurement starts when a trigger event is received.
Equivalent command:INITiate[1][:IMMediate]

Query: Not supported

Setting: :INITiate[:IMMediate]:SEQuence[1]

Example: INIT:SEQ — Set 87235 to Wait for Trigger state.

Reset state: None

:INPut:TRIGger:IMPedance

Function: Query or set the trigger input impedance.
Note: The 87235 does not support this command at the moment. This command is used for expansion.

Query: INPut:TRIGger:IMPedance?

Setting: INPut:TRIGger:IMPedance <character data>
Valid forms of character data:
LOW or 0: 50Ω
HIGH or 1: 100kΩ

Example: INP:TRIG:IMP? — Query the input impedance

INP:TRIG:IMP HIGH — Set the input impedance to high (100kΩ)

Reset LOW

state:

:OUTPut:TRIGger[:STATe]

Function: Query or set the trigger output enable state.
The "Trigger Output" port has the following commands associated with it:
:SERVice:BIST:TBASe:STATe
:SERVice:BIST:VIDeo:STATe
Since there is only one trigger output port, the last input signal of the trigger output port is based on the most recently opened signal, and the other states are switched to "OFF".

Query: :OUTPut:TRIGger[:STATe]?

Setting: :OUTPut:TRIGger[:STATe] <Boolean data>
Valid forms of <Boolean data> are: 0, OFF, 1, ON.

Example: OUTP:TRIG 0 Disable trigger output.

Reset state: None

:TRIGger[1][:IMMediate]

Function: This command puts the 87235 in the trigger waiting state immediately.
The equivalent command is :
INITiate[1]:[IMMediate]
TRIGger[:SEQuence[1]][:IMMediate]

Query: Not supported

Setting: :TRIGger[1][:IMMediate]

Example: TRIG Place the 87235 in the trigger waiting state immediately.

Reset state: None

:TRIGger:MODE

Function: Query or set the trigger mode of the 87235.

Query: :TRIGger:MODE?

Setting: :TRIGger:MODE <AUTO|NORMal|ALEVel|0|1|2>
AUTO or 0 used to set the automatic trigger mode (If no trigger signal is detected, the 87235 will still be able to measure, but the waveform display may be unstable.) ;
NORMal or 1 used to set the normal trigger mode (if no trigger signal is detected, the 87235 stops measuring until a trigger signal is detected again).
LEVel or 2 used to set the auto-level trigger mode (if no trigger signal is detected, the 87235 automatically searches for the trigger level). ALEVel consists of AUTO and LEVEL jointly.

Example: TRIG:MODE? Query trigger mode (0 means AUTO, 1 means NORMal, 2 means ALEVel).

TRIG:MODE AUTO Set to Auto-Trigger.

Limit: None.

Reset state: The trigger mode is set to Auto-Trigger.

:TRIGger[:SEQuence[1]]:COUNt

Function: Query or set the number of trigger event detection/measurement cycles.

For example, a trigger count of 100 means that 100 measurements need to be performed in order to respond to 100 triggers.

The "CALibration[1]:ZERO:AUTO" is set to auto-zero OFF when the number of trigger settings exceeds 1.

When "CALibration[1]:ZERO:AUTO" is set to auto-zero ON, the trigger count returns to the default value of 1.

Query: :TRIGger[:SEQuence[1]]:COUNt? [MIN|MAX]

Setting: :TRIGger[:SEQuence[1]]:COUNt <numeric data>

Valid values for numeric data are: DEF, MIN, MAX, <NRf>, where DEF and <NRf> are used for setting only.

<NRf> ranges from 1 to 500.

DEF is 1,

MIN is 1,

MAX 为 500.

Example:

TRIG:COUN?	Query the trigger times.
TRIG:COUN? MIN	Query the minimum settable trigger times.
TRIG:COUN 100	Set the trigger count to 500.
TRIG:COUN DEF	Set the trigger count to the default value (1 time).

Error message: If the current [SENSe[1]:]MRATe is not in FAST, it prompts "-221, "Settings conflict"";

Reset state: trigger times is 1.

:TRIGger[:SEQuence[1]]:DELay

Function: Query or set the trigger delay.

Query: :TRIGger[:SEQuence[1]]:DELay? [MIN|MAX]

Setting: :TRIGger[:SEQuence[1]]:DELay <numeric data>

Valid values for numeric data are: DEF, MIN, MAX, <NRf>, where DEF and <NRf> are used for setting only.

<NRf> ranges from -1 to +1, in seconds,

DEF is 0,

MIN is -1,

MAX is +1.

Example:

TRIG:DEL?	Query the trigger delay.
TRIG:DEL? MIN	Query the minimum settable trigger delay.

TRIG:DEL 1E-4	Set the trigger delay to 100us.
TRIG:DEL DEF	Set the trigger delay to the default value (0 second).

Limit: None.

Description: None.

Reset state: Trigger delay is set to 0 second.

:TRIGger[:SEQuence[1]]:HOLDoff

Function: Query or set the holdoff of the 87235, in seconds.

Query: :TRIGger[:SEQuence[1]]:HOLDoff? [MIN|MAX]

Setting: :TRIGger[:SEQuence[1]]:HOLDoff <numeric data>

Valid values for numeric data are: DEF, MIN, MAX, <NRf>, where DEF and <NRf> are used for setting only.

<NRf> ranges from 1e-6 to 1 and DEF is 1e-6.

Example:	TRIG:HOLD?	Query the current trigger holdoff.
	TRIG:HOLD 0.01	Set the holdoff to 10ms.

Limit: None

Reset state: Holdoff is set to 1e-6 seconds.

:TRIGger[:SEQuence[1]]:IMMediate

Function: This command puts the 87235 in the trigger waiting state immediately.

The equivalent command is:INITiate[1]:[IMMediate]

TRIGger[1][:IMMediate]

Query: Not supported

Setting: :TRIGger[:SEQuence[1]]:IMMediate

Example:	TRIG:IMM	Place Channel A in the trigger waiting state immediately.

Limit: None

Reset state: None

:TRIGger[:SEQuence[1]]:POSition

Function: Query or set the delay of the trigger event relative to the initial measurement. Assuming that the trigger delay time is zero, set the trigger position to LEFT without delay, set to RIGHT will delay 10 horizontal scales, and set to MIDDLE to delay 5 horizontal scales. Note that the TRIGger:DELay command affects the position of the triggered event.

Query: :TRIGger[:SEQuence[1]]:POSition?

The return value is 0 to 2, indicating the left, center and right trigger position respectively.

Setting: :TRIGger[:SEQuence[1]]:POSition <character data>

Valid character data are:

LEFT or 0: Left trigger;
MIDDle or 1: Middle trigger;
RIGHt or 2: Right trigger.

Example:	TRIG:POS?	Query the trigger position.
	TRIG:POS MIDD	Set the trigger position to middle trigger.
	TRIG:POS 1	Set the trigger position to middle trigger.

Limit: For pulse measurement mode only

Reset state: Set the trigger position to left trigger.

:TRIGger[:SEQuence[1]]:SLOPe

Function: Query or set the trigger slope.

Query: :TRIGger[:SEQuence[1]]:SLOPe?

Setting: :TRIGger[:SEQuence[1]]:SLOPe <character data>
Valid values of character data are:
0 or POSitive: Capture the trigger event at the rising edge of the signal.
1 or NEGative: Capture the trigger event at the falling edge of the signal.

Example:	TRIG:SLOP?	Query the trigger slope.
	TRIG:SLOP NEG	Set the falling edge trigger.

Limit: None

Reset state: The trigger slope is set to rising edge trigger (POSitive).

:TRIGger[:SEQuence[1]]:SOURce

Function: Query or set the trigger source.
The equivalent command is :TRIGger[1]:SOURce

Query: :TRIGger[:SEQuence[1]]:SOURce?

Setting: :TRIGger[:SEQuence[1]]:SOURce <character data>
Valid values of character data are:
BUS: The trigger source is a "*TRG" generic command or a "TRIGger:IMMediate" SCPI command.
EXTernal: The trigger source is the trigger input on the rear panel.
HOLD: Trigger hang, trigger 87235 with "TRIGger:IMMediate" command.
IMMediate: Trigger the system to run all the time. If "INITiate:CONTinous" is set to "ON", the 87235 operates in the free-run mode, otherwise, after "INITiate:IMMediate " is sent, the 87235 enters the measurement stop state (IDLE state) after one measurement.
INTernal[1] means the trigger source is Channel A.

Example:	TRIG:SOUR?	Query the trigger source.
	TRIG:SOUR INT1	Set the trigger source to Channel A.

Reset state: Trigger source is set to Channel A (INT1).

3.3.11 Unit Subsystem Command (UNIT)

- :UNIT[1]|2|3|4:POWer 150
- :UNIT[1]|2|3|4:POWer:RATio 150

:UNIT[1]|2|3|4:POWer

Function: Query or set the specified measurement power unit. The menu operations are linear and logarithmic.

Absolute power measurements are in W and dBm, corresponding to linear and logarithmic, respectively.

Ratio measurements and relative power measurements are in % and dB, corresponding to linear and logarithmic, respectively.

UNIT1 corresponds to Measurement 1;

UNIT2 corresponds to measurement 2;

UNIT3 corresponds to measurement 3;

UNIT4 corresponds to measurement 4

Query: :UNIT[1]|2|3|4:POWer?

Setting: :UNIT[1]|2|3|4:POWer <character data>

Valid character data are:

DBM or 0: Logarithmic display.

W or 1: Linear display

Example:

UNIT2:POW?	Query the power unit of Measurement 2.
UNIT1:POW W	Set the power unit of Measurement 1 to W.

Reset state: Set to DBM

:UNIT[1]|2|3|4:POWer:RATio

Function: Query or set the specified measurement ratio measurement power unit. The menu operations are linear and logarithmic.

UNIT1 corresponds to Measurement 1;

UNIT2 corresponds to measurement 2;

UNIT3 corresponds to measurement 3;

UNIT4 corresponds to measurement 4.

Query: :UNIT[1]|2|3|4:POWer:RATio?

Setting: :UNIT[1]|2|3|4:POWer:RATio <character data>

Valid character data are:

DB or 0: Logarithmic display.

PCT or 1: Linear display (PCT indicates %)

Example:

UNIT2:POW:RAT?	Query the power unit of Measurement 2.
UNIT1:POW:RAT PCT	Set the power unit of Measurement 1 to PCT.

Reset state: Set to DB

3.3.12 Service Subsystem Command (SERVice)

- :SERVice:BIST:TBASe:STATe 151
- :SERVice:BIST:VIDeo:STATe 151
- :SERVice:SENSor[1]:CDATe? 151
- :SERVice:SENSor[1]:CPLace? 152
- :SERVice:SENSor[1]:FREQuency:MAXimum? 152
- :SERVice:SENSor[1]:FREQuency:MINimum? 153
- :SERVice:SENSor[1]:SNUMber? 153
- :SERVice:SENSor[1]:TYPE? 153
- :SERVice:SNUMber 153

:SERVice:BIST:TBASe:STATe

Function: Query or set the state of the internal 10MHz time base signal output at the "trigger output" port for debugging purposes.

The port has the following commands associated with it.

:SERVice:BIST:TBASe:STATe

:SERVice:BIST:VIDeo:STATe

:OUTPut:TRIGger:[STATe]

Since there is only one trigger output port, the last input signal of the trigger output port is based on the most recently opened signal, and the other states are switched to "OFF".

Query: :SERVice:BIST:TBASe:STATe?

Setting: :SERVice:BIST:TBASe:STATe <Boolean data>

Valid forms of <Boolean data> are: 0, OFF, 1, ON

Example: SERV:BIST:TBAS:STAT? Query the output state of the time base signal.

Example: SERV:BIST:TBAS:STAT 1 Turn on the output of the time base signal.

Error message: None

Reset state: OFF

:SERVice:BIST:VIDeo:STATe

Function: Query or set the state of video output signal output at the "trigger output" port for debugging purposes.

The port has the following commands associated with it.

:SERVice:BIST:TBASe:STATe

:SERVice:BIST:VIDeo:STATe

:OUTPut:TRIGger:[STATe]

Since there is only one trigger output port, the last input signal of the trigger output port is based on the most recently opened signal, and the other states are switched to "OFF".

Query: :SERVice:BIST:VIDeo:STATe?

Setting: :SERVice:BIST:VIDeo:STATe <Boolean data>
Valid forms of <Boolean data> are: 0, OFF, 1, ON

Example: SERV:BIST:VID:STAT? Query the output state of the video output.

SERV:BIST:VID:STAT 1 Turn on the output of the video output.

Error message: None

Reset state: OFF

:SERVice:SENSor[1]:CDATe?

Function: Query the calibration date of the 87235. The calibration date is stored in the EEPROM of the 87235.

Query: :SERVice:SENSor[1]:CDATe?

Setting: Not supported

Example: SERV:SENS:CDAT? Query the calibration date of the 87235.

Error message: None

Reset state: None.

:SERVice:SENSor[1]:CPLace?

Function: Query the calibration address of the 87235. The calibration address is stored in the EEPROM of the 87235.

Query: :SERVice:SENSor[1]:CPLace?

Setting: Not supported

Example: SERV:SENS:CPL? Query the calibration address of the 87235.

Error message: None

Reset state: None.

:SERVice:SENSor[1]:FREQuency:MAXimum?

Function: Query the maximum frequency of the 87235. The maximum frequency is stored in the EEPROM of the 87235.

Query: :SERVice:SENSor[1]:FREQuency:MAXimum?

Setting: Not supported

Example: SERV:SENS:FREQ:MAX? Query the maximum frequency of the 87235.

Error message: None

Reset state: None.

:SERVice:SENSor[1]:FREQuency:MINimum?

Function: Query the minimum frequency of the 87235. The minimum frequency is stored in the EEPROM of the 87235.

Query: :SERVice:SENSor[1]:FREQuency:MINimum?

Setting: Not supported

Example: SERV:SENS:FREQ:MIN? Query the minimum frequency of the 87235.

Error message: None

Reset state: None.

:SERVice:SENSor[1]:SNUMber?

Function: Query the string number of the 87235. The string number of the 87235 is stored in the EEPROM of the 87235.

Query: :SERVice:SENSor[1]:SNUMber?

Setting: Not supported

Example: SERV:SENS:SNUM? Query the string number of the 87235.

Error message: None

Reset state: None.

:SERVice:SENSor[1]:TYPE?

Function: Query the type of the 87235. The type of the 87235 is stored in the EEPROM of the 87235.

Query: :SERVice:SENSor[1]:TYPE?

Setting: Not supported

Example: SERV:SENS:TYPE? Query the type of the 87235.

Error message: None

Reset state: None.

:SERVice:SNUMber

Function: Query or set the string number of the 87235.

Query: :SERVice:SNUMber?

Setting: :SERVice:SNUMber <character data>
Temporarily reserved.

Example: SERV:SNUM?

Error message:	None
Reset state:	None.

4. Programming Examples

- Basic Operation Examples.....155
- Advanced Operation Examples.....160
- Application Examples.....165

4.1 Basic Operation Examples

Take the following as an example to describe the basic method for realizing instrument program control programming via the VISA library. Take the C++ language as an example.

- VISA Library.....155
- Example Runtime Environment.....156
- Initialize and Set Default State.....157
- Send Setting Command.....158
- Read the State of Measuring Instrument.....158
- Command Synchronization.....159

4.1.1 VISA Library

VISA is the generic name for the standard I/O function library and its associated specifications. VISA library function is a set of functions that can be easily called. Its core function can control various types of devices without considering the interface type of devices and the use of different I/O interface software. These library functions are used to write the driver program of the instrument and complete the command and data transmission between the computer and the instrument, so as to realize program control of the instrument. By initializing the addressing string ("VISA resource string"), a connection to an instrument with a program port (LAN, USB, GPIB and RS-232, etc.) can be established.

To achieve remote control, it is first required to install the VISA library. VISA library packages the underlying transmission functions of VXI, GPIB, LAN and USB interfaces to make it convenient for users to recall directly. The programming interface supported by the 87235 is USB. These interfaces, combined with the VISA library and programming language, allow remote control of the 87235. At present, Keysight I/O Library provided by Keysight is often used as the underlying I/O Library.

Figure 4.1 shows the relationship between the program control interfaces, VISA libraries, programming languages and the 87235 with the USB interface as an example.

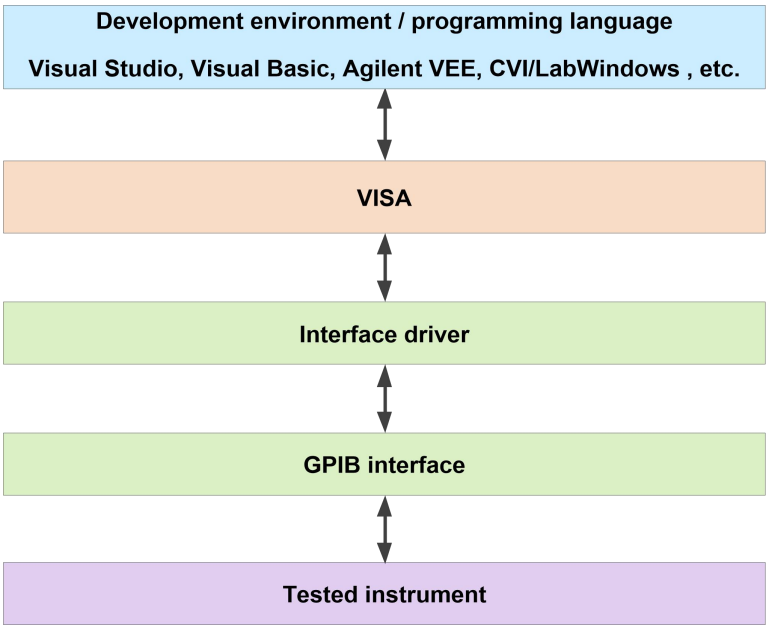


Fig.4.1 Programmable software/hardware layer

4.1.2 Example Runtime Environment

4.1.2.1 Configuration Requirements

The programming examples described in this chapter have run successfully on a computer configured as follows.

IBM compatible PC above Pentium class;

Windows 2000, Windows XP, Windows 7 or, Windows 8, Windows 10 operating systems.

Visual Studio 2010/2012/2013/2015/2017 integrated development environment;

VISA library of NI or Keysight;

USB cable

4.1.2.2 Files Included

To run an example program written in C/C++, you must include the required files in the VC project.

If you use the VISA library, you must:

Add visa32.lib to the source file;

Add visa.h to the header file.

If you use the NI-488.2 library, you must:

Add GPIB-32.OBJ file to the source file;

Add windows.h file to the header file;

Add Deci-32.h file to the header file.

For more information about the NI-488.2 library and VISA library, please refer to the websites of NI and Keysight respectively.

4.1.3 Initialize and Set Default State

To start the program, the VISA resource manager must be initialized, so as to open and establish the communication connection between the VISA library and instrument. The specific steps are as follows:

4.1.3.1 Generate Global Variables

Start by generating global variables that other program modules will recall, such as instrument handle variables. The following example programs should contain the following global variables:

ViSession iDevHandle;

ViSession iDefaultRM;

const char rgcDevRsc[MAX_RSC_LEN] = "USB0::0x3399::0x3810::2019001::0::INSTR";

const int iTmo = 5000;

Where, the constant rgcDevRsc represents the instrument descriptor, "USB0" represents the controller, "0x3399" represents the vendor ID of the instrument, 0x3810 is the product ID, and 2020001 is the product serial number.

If the instrument is controlled via the GPIB interface and the GPIB address is "20", then the value of the variable is

const char rgcDevRsc[MAX_RSC_LEN] = "GPIB0::20::INSTR";

If the instrument is controlled via a LAN socket interface with IP address 192.168.1.1 and port number 5025, then the value of the variable is

const char rgcDevRsc[MAX_RSC_LEN] = "TCPIP0::192.168.1.1::5025::SOCKET";

If the instrument is controlled via the LAN interface with IP address 192.168.1.1, then the value of the variable is

const char rgcDevRsc[MAX_RSC_LEN] = "TCPIP0::192.168.1.1::INSTR";

4.1.3.2 Initialize the Controller

/**

The following example shows the way to open and establish the communication connection between the VISA library and instrument (with instrument descriptor specified).

//Initialize the master: open the default resource manager and return the instrument handle iDevHandle.

**/

void InitController()

{

ViStatus iStatus;

iStatus = viOpenDefaultRM(&iDefaultRM);

iStatus = viOpen(iDefaultRM, rgcDevRsc, VI_NULL, VI_NULL, &iDevHandle);

}

4.1.3.3 Initialize the instrument

/***/

The following examples show how to initialize the default state of the instrument and empty the status register.

/***/

```
void InitDevice()
{
ViStatus iStatus;
ViUInt32 uiRetCnt;
iStatus = viWrite(iDevHandle, "*CLS\n", strlen("*CLS\n"), &uiRetCnt); //Status Reset
iStatus = viWrite(iDevHandle, "*RST\n", strlen("*RST\n"), &uiRetCnt); //Instrument Reset
}
```

4.1.4 Send Setting Command

/***/

The following example shows how to set the frequency of the 87235.

/***/

```
void SimpleSettings()
{
ViStatus iStatus;
ViUInt32 uiRetCnt;
//Set the frequency to 128MHz
iStatus = viWrite(iDevHandle, "FREQ 1.2e8\n", strlen("FREQ 1.2e8\n"), &uiRetCnt);
}
```

4.1.5 Read the State of Measuring Instrument

/***/

The following examples show how to read the set state of the instrument.

/***/

```
void ReadSettings()
{
    ViStatus iStatus; //Status
    ViUInt32 uiRetCnt; //read the returned bytes
    char rgcBuf[256]; //Temporary buffer
    char* pcCmd = NULL; //Command pointer

    //QueryFreq
```

```
    pcCmd = "FREQ?\n";
    iStatus = viWrite(iDevHandle, pcCmd, strlen(pcCmd), &uiRetCnt);
    Sleep(10);
    iStatus = viRead(iDevHandle, rgcBuf, sizeof(rgcBuf), &uiRetCnt);
    //Print debugging information
    printf("frequency %s", rgcBuf);
}
```

4.1.6 Command Synchronization

```
/*************************************************************************/
```

The following examples illustrate the methods for command synchronization with sweep process.

```
/*************************************************************************/
void SweepSync()
{
    ViStatus iStatus; //Status
    ViUInt32 uiRetCnt; //read the returned bytes
    ViEventType eType; //Event Type
    ViEvent eEvent; //Event
    int iStat; //Status word
    char rgcOpcOk[256]; //OPC string
    char* pcCmd = NULL; //Command pointer

    /*************************************************************************/
    /* The command INITiate[:IMMediate] is used to start single sweep (when continuous sweep is OFF, INIT:CONT OFF)*/
    /* Only at the end of single sweep can the next command in the command buffer be executed */ */
    /*************************************************************************/
    pcCmd = "INIT:CONT OFF\n";
    iStatus = viWrite(iDevHandle, " pcCmd ", strlen(pcCmd), &uiRetCnt);
    //Method 1 for waiting for the sweep to end: use *WAI
    pcCmd = "ABOR;INIT:IMM;*WAI\n";
    iStatus = viWrite(iDevHandle, " pcCmd ", strlen(pcCmd), &uiRetCnt);
    //Method 2 for waiting for the sweep to end: use *OPC
    pcCmd = "ABOR;INIT:IMM; *OPC?\n";
```

```
    iStatus = viWrite(iDevHandle, " pcCmd ", strlen(pcCmd), &uiRetCnt);
    iStatus = viRead(iDevHandle, rgcOpcOk, 2, &uiRetCnt); //wait for *OPC to return “1”
    //Main program continues……
}
```

4.2 Advanced Operation Examples

- USBTMC Program Control Example……160
- Linux development examples……160

4.2.1 USBTMC Program Control Example

- Before Using the Examples……160
- Example……160

4.2.1.1 Before Using the Examples

If you use VISA library for program control, you need to install VISA library, such as KeysightIO17.2, NI VISA5.0, etc.

Note that lower versions of the VISA library do not support the USBTMC programming feature.

4.2.1.2 Examples

- Using VISA library and C++ language to implement web……160

1) Using VISA library and C++ language to implement web programs

```
/*************************************************************
In this example, USB program control is implemented via the VISA library.
Start VS2005 or above, add the necessary files and add the directory where visa.h is located to the "Include files" path of the project (to add: press "Tools" in the menu, then press "Options", "Projects and Solutions", "VC++ Directory", and then select "Include files" under the "Show directories with the following content", and add the directory where visa.h is located in the list. (For the English version of VS, please refer to the above method to set up, without further explanation.)
Enter the following code into your .cpp file
*************************************************************/
#include "stdafx.h"
#include <visa.h>
#include <stdio.h>
#include <stdlib.h>

#define M_USB_VID     1204       //USB Vendor ID
#define M_USB_PID     4112       //Instrument ID
#define M_USB_SN      "ZGK00541" //Instrument Serial Number (No.)
```

```
//Description:
ViSession g_uiDefaultRm = 0; //Resource Handle
ViSession g_uiInstrHandle = 0; //Device VISA Handle

void UsbInit(void);
void UsbTest(void);
void UsbClose(void);
//USB test main program
void UsbTestMain(void)
{
    //Initialize (user opens the instrument connection before using the instrument)
    UsbInit();

    //Test (user can communicate with the instrument)
    UsbTest();

    //OFF (close the instrument connection when the user is no longer using the
instrument)
    UsbClose();
}

//USB initialization
void UsbInit(void)
{
    ViStatus iStatus = 0; //Status
    ViChar rgcBuf[256]; //Temporary Buffer

    sprintf(rgcBuf, "USB0::%d::%d::%s::0::INSTR", M_USB_VID,M_USB_PID,M_USB_SN);
    iStatus = viOpenDefaultRM(&g_uiDefaultRm); //Open VISA Task
    if (iStatus)
    {
        printf("The task cannot be opened. Please recheck the device and connect\n").
    }
    else
    {
```

```
        iStatus = viOpen(g_uiDefaultRm, rgcBuf, VI_NULL, 5000, &g_uiInstrHandle);
        if (iStatus)
        {
            printf("The devicee cannot be opened. Please recheck the device and
connect\n");
        }
        else
        {
        }
    }
}
//USB Test
void UsbTest(void)
{
    ViStatus iStatus = 0; //Status
    ViChar rgcBuf[256]; //Temporary Buffer
    ViByte rgcRead[256]; //Read buffer
    ViReal64 rgdFreq[2]; //Frequency array
    ViUInt32 uiRetCnt; //Return length

    if (0 == g_uiInstrHandle)
    {
        printf("The device is not opened. Please recheck the device and connect\n");
    }
    else
    {
        //1) First query the frequency of Channel A, and store it in rgdFreq[0]
        viPrintf(g_uiInstrHandle, "SENS1:FREQ?\n");
        Sleep(10);
        viRead(g_uiInstrHandle, rgcRead, sizeof(rgcRead), &uiRetCnt);
        rgcRead[uiRetCnt] = 0;
        printf((PCHAR)rgcRead);

        sscanf((PCHAR)&rgcRead[0], "%lf", &rgdFreq[0]);
        sprintf(rgcBuf, "Frequency of Channel A: %lg\n", rgdFreq[0]);
```

```
            printf(rgcBuf);

            //2) Set the frequency of Channel A to .78GHz
            viPrintf(g_uiInstrHandle, "SENS1:FREQ    %lfGHz\n", 16.78);

            //3) Query the frequency of Channel A, and store it in rgdFreq[1]
            viPrintf(g_uiInstrHandle, "SENS1:FREQ?\n");
            viScanf(g_uiInstrHandle, "%t", rgcBuf);            //Put the query results into an
array
            printf(rgcBuf);

            sscanf(rgcBuf, "%lf", &rgdFreq[1]);
            sprintf(rgcBuf, "Frequency of Channel A: %lg\n", rgdFreq[1]);
            printf(rgcBuf);

            //4) Restore the frequency of Channel A
            viPrintf(g_uiInstrHandle, "SENS1:FREQ    %lg\n", rgdFreq[0]);
        }
}
//USB close
void UsbClose(void)
{
    if (0 != g_uiInstrHandle)
    {
        viClose(g_uiInstrHandle); //Close the device
        g_uiInstrHandle = 0;
    }
    if (0 != g_uiDefaultRm)
    {
        viClose(g_uiDefaultRm); //Close default tasks
        g_uiDefaultRm = 0;
    }
}
```

4.2.2 Linux development examples

Currently, there are many versions of Linux systems in the market, and most of them cannot install the VISA library. The example in this section uses the system common read/write command to realize the programmable use of the 87235.

Note: Linux should support the USBTMC protocol.

```
**************************************************************************

#include <fcntl.h>


#define O_RDWR                  2
#define USB_MAX_BUFFER     4096
#define M_CMD_IDN             "*IDN?"
#define M_CMD_MEASURE       "MEAS?"


int UsbtmcTest()
{
    //If there are multiple devices, it may be "/dev/usbtmc1",.....
    char* pcUsbtmcDev = "/dev/usbtmc0";
    char* pcWritePtr;
    unsigned int uiHandle;
    unsigned long dwReadCnt;
    char cReadBuf[USB_MAX_BUFFER];
    unsigned int iStatus;

    //The device must be turned on before use
    uiHandle = open(pcUsbtmcDev, O_RDWR, 666);

    //Send the command "*IDN?" to the device
    pcWritePtr = M_CMD_IDN;
    iStatus = write(uiHandle, pcWritePtr, strlen(pcWritePtr));
    //Read information from the device
    dwReadCnt = read(uiHandle, cReadBuf, USB_MAX_BUFFER);
    printf("IDN is: %s", cReadBuf);

    //Send the command "MEAS?" to the device
    pcWritePtr = M_CMD_MEASURE;
```

```
    iStatus = write(uiHandle, pcWritePtr, strlen(pcWritePtr));
    //Read information from the device
    dwReadCnt = read(uiHandle, cReadBuf, USB_MAX_BUFFER);
    printf("The measurement result is : %s", cReadBuf);

    //The device must be turned off at the end of use
    close(uiHandle);
}
************************************************************************
```

4.3 Application Examples

4.3.1 Fast build-up of top-of-pulse average power measurements with "gates"

- SYST:PRES //Reset the device to its default value
- DET:FUNC NORM //Set the measurement mode to "NORM"
- TRIG:SOUR INT //Trigger source set to internal
- TRAC:STAT ON //Enable trace measurement
- SENS:FREQ 1GHz //Set the frequency to 1GHz
- CALC:FEED "POW:AVER ON SWEEP1" //Configure Measurement 1 to measure the average power of Gate 1
- SENS:TRAC:AUTO //Automatic setting
- SENS:SWE:AUTO:REF1 10.0 //Set the start position of automatic gate to 10% of Gate 1
- SENS:SWE:AUTO:REF2 10.0 //Set the end position of automatic gate to 90% of Gate 1
- SENS:SWE:AUTO ON //Set Gate 1 as automatic gate
- MEAS? //Perform one measurement and obtain the average power of Gate 1

4.3.2 GSM timeslot measurements in list mode

- DET:FUNC NORM //Set the measurement mode to "NORM"
- TRIG:SOUR EXT //Trigger source set to external
- SENS:LIST:STAT ON //Enable list mode.
- SENS:LIST:FREQ:STAR 1GHz //Set start frequency to 1GHz
- SENS:LIST:FREQ:STOP 10GHz //Set start frequency to 10GHz
- SENS:LIST:POIN 10 //Set the number of measurement points to 10
- SENS:LIST:MTYP AVER //Set the measurement type to average power
- SENS:LIST:TSC 2 //Set the number of time slots to 2

- SENS:LIST:TSL:EXCL:OFFS:TIME 0 //Offset time of the exclusion area is 0
- SENS:LIST:TSL:EXCL:TIME 0 //Time length of the exclusion area is 0
- SENS:LIST:TSL:TIME 577e-6 //Time length of the time timeslot measurement is 577us
- SENS:LIST:TSL:TREF1 10 //Start time offset of the time timeslot measurement is 10%

Repeat the following commands to obtain multiple measurement results

- INIT:CONT ON //Initiate measurement
- *OPC //Set the operation end bit in the standard event state register
- *ESR? //Query the value of the standard event state register
- FETC? //Fetch measurement results

4.3.3 External Trigger Buffer Measurement

- DET:FUNC NORM //Set the measurement mode to "NORM"
- TRIG:SOUR EXT //Trigger source set to external
- SENS:FREQ 1GHz //Set the frequency to 1GHz
- SENS:FREQ:STEP 0 //Sweep points 0
- SENS:BUFF:MTYP "AVER" //Buffer measurement type is Average Power
- SENS:BUFF:COUN 10 //Number of buffer measurements 10
- SENS:SWE:OFFS:TIME 100e-6 //Time offset relative to trigger position 100us
- SENS:SWE:TIME 800e-6 //Time length of measurement 800us

Repeat the following commands to obtain multiple measurement results

- INIT:CONT ON //Initiate measurement
- *OPC //Set the operation end bit in the standard event state register
- *ESR? //Query the value of the standard event state register
- FETC? //Fetch measurement results

4.3.4 External Trigger Buffer Sweep Measurement

- DET:FUNC AVER //Set the measurement mode to "AVER"
- TRIG:SOUR EXT //Trigger source set to external
- SENS:FREQ:STAR 1GHz //Set the start frequency to 1GHz
- SENS:FREQ:STOP 10GHz //Set start frequency to 10GHz
- SENS:FREQ:STEP 10 //Sweep points 10
- SENS:SWE:APER 100e-6 // Set the aperture length to 100us
- TRIG:DEL 10e-6 // Set the trigger delay to 10us

Repeat the following commands to obtain multiple measurement results

- INIT:CONT ON //Initiate measurement
- *OPC //Set the operation end bit in the standard event state register
- *ESR? //Query the value of the standard event state register
- FETC? //Fetch measurement results

4.3.5 Fast Measurement Mode (Free Run)

"AVER" mode (50000 readings/sec)

- SYST:PRES //Reset the device to its default value
- SENS:FREQ 1GHz //Set the frequency to 1GHz
- UNIT:POW W //Calculation 1 power measurement unit W
- SENS:AVER:SDET OFF //Step detection OFF
- SENS:AVER OFF //Measurement average OFF
- SENS:DET:FUNC AVER //Measurement mode "AVER"
- SENS:MRAT FAST //Measurement speed in fast mode
- TRIG:COUN 200 //Measurement buffer size 200
- SENS:SWE:APER 20e-6 //Set the aperture length to 20us
- FETC? //Fetch measurement results

4.3.6 Fast Measurement Mode (External Trigger)

When the aperture length is not larger than the time interval of the external trigger signal, the external trigger signal can be captured continuously without interruption.

The measurement speed is determined by the greater of the time interval of the external trigger signal and the length of the aperture, with max 50000 readings/second.

The following routines help users establish GSM timeslot measurement based on external trigger (16 GSM Architecture), which can continuously measure 128 timeslots.

- SYST:PRES //Reset the device to its default value
- SENS:FREQ 1GHz //Set the frequency to 1GHz
- TRIG:SOUR EXT //Set to external trigger
- SENS:AVER:SDET OFF //Step detection OFF
- SENS:AVER OFF //Measurement average OFF
- SENS:DET:FUNC AVER //Measurement mode "AVER"
- SENS:MRAT FAST //Measurement speed in fast mode
- TRIG:COUN 128 //Measurement buffer size 128
- TRIG:DEL 50e-6 //Set the trigger delay to 50us
- SENS:SWE:APER 500e-6 //Set the aperture length to 500us

- FETC? //Fetch measurement results

4.3.7 Continuous and Uninterrupted Measurements

The average power of known periodic signals, especially large periodic signals, can be accurately measured.

Mode 1: Accurate measurement of the signal with a period of 5s = 50ms*100 (FETCH mode)

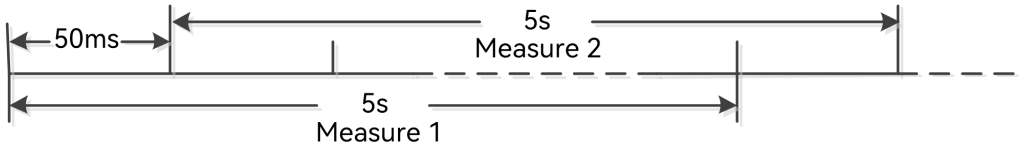


Figure 4.1 Measurement process diagram

- SYST:PRES //Reset the device to its default value
- SENS:FREQ 1GHz //Set the frequency to 1GHz
- CAL:ZERO:AUTO OFF //Auto-Zero OFF
- CAL:AUTO OFF //Auto-Calibration OFF
- SENS:AVER:SDET OFF //Step detection OFF
- SENS:DET:FUNC AVER //Measurement mode "AVER"
- SENS:SWE:APER 50e-3 //Set the aperture measurement length to 50ms
- SENS:AVER:COUN 100 //Set the average number of measurements to 100

  // Delay 5s
- FETC? //Fetch measurement results

Mode 2: Accurate measurement of the signal with a period of 5s = 50ms*100 (MEAS mode)

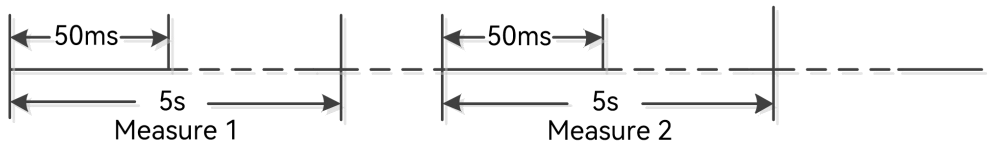


Figure 4.2 Measurement process diagram

- SYST:PRES //Reset the device to its default value
- SENS:FREQ 1GHz //Set the frequency to 1GHz
- CAL:ZERO:AUTO OFF //Auto-Zero OFF
- CAL:AUTO OFF //Auto-Calibration OFF
- SENS:AVER:SDET OFF //Step detection OFF
- SENS:DET:FUNC AVER //Measurement mode "AVER"
- SENS:SWE:APER 50e-3 //Set the aperture measurement length to 50ms
- SENS:AVER:COUN 100 //Set the average number of measurements to 100

- MEAS? //Perform a measurement and obtain the results

Mode 3: Accurate measurement of the signal with a period of 1s = 50ms*20 (The measurement period of this method cannot exceed 1 second)

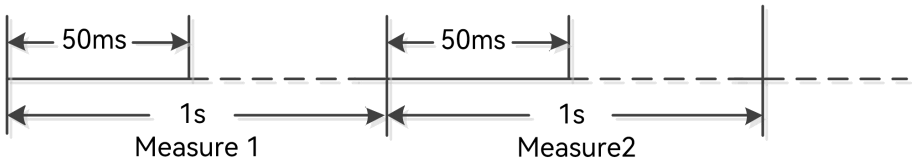


Figure 4.3 Measurement process diagram

- SYST:PRES //Reset the device to its default value
- SENS:FREQ 1GHz //Set the frequency to 1GHz
- CAL:ZERO:AUTO OFF //Auto-Zero OFF
- CAL:AUTO OFF //Auto-Calibration OFF
- SENS:AVER OFF //Measurement average OFF
- SENS:AVER:SDET OFF //Step detection OFF
- SENS:DET:FUNC AVER //Measurement mode "AVER"
- SENS:MRAT FAST //Measurement speed in fast mode
- TRIG:COUN 20 //Measurement buffer size 20
- SENS:SWE:APER 50e-3 //Set the aperture measurement length to 50ms
- FETC? //Obtain the measurement results (the average power in this period can be obtained by summing and averaging all the measurement results)

5. Error Description

This chapter will show you how to find problems and accept after-sales service, and explain error message of the 87235.

- Error Message.....171
- Repair Methods.....175

5.1 Error Message

The 87235 records errors during measurement in two ways: error message queues displayed on the front panel and SCPI (in the remote control mode) error message queues. which are stored and managed separately.

1) Error message format and description

In remote control mode, errors are recorded in the error/event queue of the status reporting system, and can be queried with the command "SYSTem:ERRor?". The format is as follows:

"<Error code>, "<Error in error queue>; ["Detailed error description]"

Example:

“-110,"Data out of range;”

The program control error message includes two types:

A negative error code defined by the SCPI standard. This type of error message is not specified here.

Table 5.1 List of descriptions on instrument feature error messages

Failure code	Error Description
-101	Invalid character Invalid character: There are invalid characters in the command string (command or parameter). For example: AVER:COUN !6
-102	Syntax error Syntax error: The command string syntax is invalid. For example: DISPlay:ACT, CH1
-108	Parameter not allowed Parameters are not allowed: the command has too many parameters, or the command without parameters follows the parameters. For example: TRAC:AUT ON
-109	Missing parameter Missing parameters: The command has too few parameters. For example: AVER
-112	Program mnemonic too long Command string is too long: A single segment of the command has more than 12 characters. For example: OUTPutROSCillatorSTATe ON

Failure code	Error Description
-113	Undefined header Undefined header: 87235 receives an unrecognized command. Possible causes: Wrong spelling, or wrong abbreviation of the command, etc. For example: CALI:AUTO
-121	Invalid character in number Invalid characters in the numeric value: there are invalid characters in the numeric parameter. For example:SENS:CORR:GAIN2 #12
-123	Exponent too large The index is too large: the index of numerical parameters exceeds 32000. For example: SENS:CORR:GAIN2 1E32001
-124	Too many digits Too many bits: the number of bits of numeric parameters exceeds 255, without the leading 0.
-128	Numeric data not allowed Numeric parameters are not allowed: commands that cannot receive numeric parameters receive a numeric value.
-131	Invalid suffix Invalid suffix: the suffix of numeric parameter is incorrect. For example: FREQ 10GZ
-134	Suffix too long Suffix too long: the suffix exceeds 12 characters. For example: FREQ 10GHHHHHHHHHHHHHHHHHHZ
-138	Suffix not allowed Suffix not allowed: numeric parameters cannot be followed by suffixes. For example: SENS:CORR:GAIN2 12HZ
-148	Character data not allowed Character data is not allowed: check whether quotation marks need to be added. For example: MEM:CLE State_1 Correct: MEM:CLE "State_1"
-151	Invalid string data Invalid string data: check whether the single quotation marks or double quotation marks of the string match. For example: MEM:CLE “State1
-158	String data not allowed Character data is not allowed: check whether the parameter type is valid. For example: OUTP:ROSC "ON"
-161	Invalid block data Invalid block data: Check according to Section 7.7.6 of IEEE 488.2.
-168	Block data not allowed

Failure code	Error Description
	Block data not allowed: a valid data block was detected, but the command does not support data blocks. For example: OUTP:ROSC #15FETC?
-178	Expression data not allowed Expression data not allowed: a valid expression was detected, but expression is not allowed in the 87235. For example: SENS:CORR:GAIN2 (1+3)
-211	Trigger ignored Trigger ignored: when 87235 is not in Wait for Trigger state, trig:imm, *trg and other commands are received.
-213	Init ignored Initialization is ignored: when 87235 has been initialized, the measurement initialization command is received. For example: INIT:CONT ON INIT
-214	Trigger deadlock Trigger deadlock
-220	Parameter error; Frequency list must be in ascending order. Parameter error; the frequency list must be arranged in ascending order
-221	Settings conflict Setting conflict: there are many reasons for conflict, such as setting trigger delay during statistical measurement.
-222	Data out of range Data out of range: Numerical data is not within the valid range. for example: AVER:COUN 100000
-224	Illegal parameter value Illegal parameter value: a discrete parameter was received, but it is invalid for this command.
-226	Lists not same length List length is different
-230	Data corrupt or stale; Please calibrate Invalid or damaged data; Please calibrate.
-231	Data questionable; CAL ERROR Data question; Calibration error: the 87235 calibration failed. The most likely reason is that 87235 is not connected to the output of the calibration source during calibration. Data questionable; CAL ERROR Ch1 Data question; Channel A calibration error: the 87235 calibration failed. The most likely reason is that 87235 is not connected to the output of the calibration source during calibration. Data questionable; CAL ERROR Ch2 Data question; Channel B calibration error: the 87235 calibration failed. The

Failure code	Error Description
	most likely reason is that 87235 is not connected to the output of the calibration source during calibration. Data questionable; Input Overload Data question; Input overload: the power input exceeds the upper power limit of the 87235. Data questionable; Input Overload Ch1 Data question; Input overload: the power input exceeds the upper power limit of the 87235. Data questionable; Lower window log error Data question; Logarithm error in lower measurement: when the difference measurement is carried out, the measurement result is 0 and the unit of display is logarithm. Data questionable; Upper window log error Data question; Logarithm error in upper measurement: when the difference measurement is carried out, the measurement result is 0 and the unit of display is logarithm. Data questionable; ZERO ERROR Data question; Zeroing error: the 87235 zeroing failed. The most likely reason is that there is power signal input during zeroing. Data questionable; ZERO ERROR Ch1 Data question; Channel A zeroing error: the 87235 zeroing failed. The most likely reason is that there is power signal input during zeroing.
-241	Hardware missing Missing hardware: 87235 cannot execute the command, type mismatch.
-310	System error; Sensor EEPROM Read Failed - critical data not found or unreadable System error; EEPROM read failed - key data not found or unreadable System error; Sensor EEPROM Read Failed - unknown EEPROM table format System error; EEPROM read failed - unknown EEPROM format.
-321	Out of memory Exceeding memory
-330	Self-test Failed; The self-test fails.
-350	Queue overflow Queue overflow: the error queue is full, and subsequent errors will no longer be recorded.
-410	Query INTERRUPTED The query is interrupted: A command needs to send data to the output buffer, but the send buffer already contains the data sent by the previous command (without overwriting the previous data). The output buffer is cleared on shutdown or on receipt of the *RST command. Refer to Section 6.3.2.3 of IEEE 488.2 for details.
-420	Query UNTERMINATED Query not ended: The 87235 is set to Speak (i.e., send data to the interface

Failure code	Error Description
	bus), but the command to send data to the output buffer is not received. Refer to Section 6.3.2.2 of IEEE 488.2 for details. For example, after executing the CONFigure command (which produces no data), an attempt is made to read data from the remote interface.
-430	Query DEADLOCKED Query deadlock: The output buffer cannot hold too much data generated by the command, and the output buffer is full. Command execution continues but data is lost. Refer to Section 6.3.1.7 of IEEE 488.2 for details.
-440	Query UNTERMINATED after indefinite response Query not ended after an indefinite response: Some combination queries may generate illegal response messages. If a query command that produces an indefinite response (any block response of indefinite length or any ASCII response data) is not the last query command, the instrument will report a query error and no further responses will be sent after that query command. Refer to Section 6.5.7.5 of IEEE 488.2 for details.

2) Error message type

The error event corresponds only to one type of error message, and the error message types are introduced in details below:

- Query error (-499 to -400): indicating that the output queue of the instrument controls and detects a message exchange protocol error described in Chapter 6 of IEEE 488.2. At this point, the query error bit (bit2) of the event status register is set (please refer to IEEE 488.2, 6.5 for details). The data cannot be successfully read from the output queue at this time.
- Instrument characteristic error (-399 to -300, 201 to 703, and 800 to 810): indicating that the instrument operation is not successful, and the reason may be abnormal hardware or firmware state. Such error codes are often used self-detection of the instrument. At this point, the instrument characteristic error bit (bit3) of the event status register is set.
- Execution error (-299 to -200): indicating that an error is detected during the measurement of the instrument. At this point, the execution error bit (bit4) of the event status register is set.
- Command error (-199 to -100): indicating a syntax error detected during command parsing of the instrument, usually due to an incorrect command format. At this point, the command error bit (bit5) of the event status register is set.

5.2 Method to Obtain After-sales Services

- Contact Us.....175
- Package and Mailing.....176

5.2.1 Contact us

In case of any failure to the 87235, check and save the error message, analyze possible causes, and refer to the methods provided in "7.2 Troubleshooting and debugging" in the User's Manual for preliminary troubleshooting. If the problem cannot be solved, contact the service and consultation center of the Company as per the contact information provided below and provide us with the error collected. We will coordinate

with you to solve the problem as soon as possible.

Contact information:

Customer service: 400-1684191

Website: www.ceyear.com

Email: techbb@ceyear.com

Postal code: 266555

Address: No. 98, Xiangjiang Road, West Coast New Area, Qingdao, Shandong, China

5.2.2 Package and mailing

In case of any failure to the 87235 that is difficult to be eliminated, contact us by phone or fax. If it is confirmed that the 87235 has to be returned for repairing, pack it with the original packing materials and case by following the steps below:

1) Prepare a detailed description of the failure of the 87235 and put it into the package along with it.

2) Pack the 87235 with the original packing materials, so as to minimize possible damage;

3) Place cushions at the 4 corners of the outer packing carton, and place the instrument in the outer packing carton.

4) Seal the opening of the packing carton with adhesive tape and reinforce the packing carton with nylon tape.

5) Specify text like "Fragile"! Do not touch! Handel with care!" and so on.

6) Please consign it as precision instruments.

7) Keep a copy of all shipping documents.

NOTICE

Precautions on packing the 87235

Using other materials for packing the 87235 may damage the instrument. Never use polystyrene beads as packing materials because on the one hand, they cannot provide sufficient protection on the instrument, and on the other hand, they can be sucked in to the instrument fan by the static electricity generated, resulting in instrument damage.

TIPS

Instrument package and transportation

Please follow carefully the precautions described in "3.1.1.1 Unpacking" of the User's Manual when transporting or handling the instrument (for example, damage occurred during delivery).

Appendixes

- Annex A Zoom Table of SCPI Classified by Subsystem.....177

Appendix A Zoom Table of SCPI Classified by Subsystem

Table 1 Zoom Table of SCPI Classified by Subsystem

Index	Command	Brief description of functions
40	*CLS	Clear the instrument status data structure
40	*DDT	Query or set the operation in response to *TRG general command. Note: The 87235 does not support this command at the moment.
41	*ESE	Query or set the standard event status enable register
42	*ESR?	Query the value of the standard event status register
42	*IDN?	Query the identification string of 87235
42	*OPC	When all waiting operations are completed, set the operation end bit in the standard event state register
42	*OPT?	Query the instrument option configuration.
43	*RCL	Call the status in the specified storage call register
43	*RST	Reset the 87235
43	*SAV	Store the instrument status into the specified register
43	*SRE	Query or set the service request register
44	*STB?	Query the status word.
45	*TRG	Trigger all channels in Wait for Trigger
45	*TST?	Perform self-test
45	*WAI	Place the 87235 in the wait state
143	:ABORt[1]	Stop the measurement of the corresponding channel of the 87235
47	:CALCulate[1]|2|3|4:FEED[1]|2	Query or set the measurement mode of measurement display
48	:CALCulate[1]|2|3|4:GAIN[:MAGNitude]	Query or set the calculation offset value in the specified measurement
48	:CALCulate[1]|2|3|4:GAIN:STATe	Query or set the switch state of the calculation offset

Index	Command	Brief description of functions
49	:CALCulate[1]|2|3|4:LIMit:CLEar:AUTO	Control when the limit FCO (failure count) is cleared
49	:CALCulate[1]|2|3|4:LIMit:CLEar[:IMMediate]	Clear the FCO (failure count) of the specified measurement
49	:CALCulate[1]|2|3|4:LIMit:FAIL?	Query whether the specified measurement exceeds the limit.
50	:CALCulate[1]|2|3|4:LIMit:FCOunt?	Query the limit detection failure count (FCO) of the specified measurement
50	:CALCulate[1]|2|3|4:LIMit:LOWer[:DATA]	Query or set the lower limit of the specified measurement limit
51	:CALCulate[1]|2|3|4:LIMit:STATe	Query or set the specified measurement limit detection switch
52	:CALCulate[1]|2|3|4:LIMit:UPPer[:DATA]	Query or set the upper limit of the specified measurement limit
53	:CALCulate[1]|2|3|4:MATH[:EXPRession]	Query or set the specified measurement expression
53	:CALCulate[1]|2|3|4:MATH[:EXPRession]:CATalogue?	Enumerate all measurement expressions
53	:CALCulate[1]|2|3|4:RELative[:MAGNitude]:AUTO	Set the reference value for relative measurement
54	:CALCulate[1]|2|3|4:RELative[:MAGNitude]:VALue?	Query the reference value for relative measurement
54	:CALCulate[1]|2|3|4:RELative:STATe	Query or set the relative measurement switch status
55	:CALibration[1][:ALL]	Zeroing and calibration of the 87235
55	:CALibration[1]:AUTO	Calibration of the 87235
56	:CALibration[1]:ZERO:AUTO	Zeroing of the 87235
56	:CALibration[1]:ZERO:TYPE	Query or set the zeroing type.
65	:CONFigure[1]|2|3|4[:SCALar][:POWer][:AC]	Query or set the power measurement mode of the specified measurement
57	:DISPlay[:WINDow[1]|2][:NUMeric[1]|2]:RESolution	Query or set the display resolution of the specified measurement
58	:FETCh[1]|2|3|4[:SCALar][:POWer][:AC]?	Set the specified measurement as absolute power measurement, turn off relative measurement, and return the measured value
58	:FETCh[1]|2|3|4[:SCALar][:POWer][:AC]:DIFFerence?	Set the specified measurement as differential power measurement, turn off relative measurement, and return the measured value
59	:FETCh[1]|2|3|4[:SCALar][:POWer][:AC]:DIFFerence:RELative?	Set the specified measurement as differential power measurement, turn on relative measurement, and return

Index	Command	Brief description of functions
		the measured value
59	:FETCh[1]|2|3|4[:SCALar][:POWer][:AC]:RATio?	Set the power measurement mode of the specified measurement as ratio measurement, turn off relative measurement, and return the measured value
60	:FETCh[1]|2|3|4[:SCALar][:POWer][:AC]:RATio:RELative?	Set the power measurement mode of the specified measurement as ratio measurement, turn on relative measurement, and return the measured value
66	:FETCh[1]|2|3|4[:SCALar][:POWer][:AC]:RELative?	Set the specified measurement as absolute power measurement, turn on relative measurement, and return the measured value
66	:FORMat[:READings]:BORDer	Query or set the transmission order of binary data
143	:FORMat[:READings][:DATA]_:\DISPlay:CLEar	Query or set the data transmission format
144	:INITiate[1]:CONTinuous	Query or set the trigger status
144	:INITiate:CONTinuous:ALL	Query or set the trigger state of all channels
145	:INITiate:CONTinuous:SEQuence[1]	Query or set the trigger status
145	:INITiate[1][:IMMediate]	Set to be in Wait for Trigger state
145	:INITiate[:IMMediate]:ALL	Set all channels to be in Wait for Trigger state
145	:INITiate[:IMMediate]:SEQuence[1]	Set to be in Wait for Trigger state
60	:INPut:TRIGger:IMPedance	Query or set the trigger input impedance. Note: The 87235 does not support this command at the moment. This command is used for expansion.
61	:MEASure[1]|2|3|4[:SCALar][:POWer][:AC]?	Set the specified measurement as absolute power measurement, turn off relative measurement, and return the measured value
61	:MEASure[1]|2|3|4[:SCALar][:POWer][:AC]:DIFFerence?	Set the specified measurement as differential power measurement, turn off relative measurement, and return the measured value
62	:MEASure[1]|2|3|4[:SCALar][:POWer][:AC]:DIFFerence:RELative?	Set the specified measurement as differential power measurement, turn on relative measurement, and return the measured value

Index	Command	Brief description of functions
62	:MEASure[1]|2|3|4[:SCALar][:POWer][:AC]:RATio?	Set the power measurement mode of the specified measurement as ratio measurement, turn off relative measurement, and return the measured value
63	:MEASure[1]|2|3|4[:SCALar][:POWer][:AC]:RATio:RELative?	Set the power measurement mode of the specified measurement as ratio measurement, turn on relative measurement, and return the measured value
67	:MEASure[1]|2|3|4[:SCALar][:POWer][:AC]:RELative?	Set the specified measurement as absolute power measurement, turn on relative measurement, and return the measured value
68	:MEMory:CATalog[:ALL]?	Enumerate the user configurations in the 87235, including storage call configuration, frequency response offset table (FDO), etc
68	:MEMory:CATalog:STATe?	Enumerate the storage call configuration in the 87235
68	:MEMory:CATalog:TABLe?	Enumerate the frequency response offset table in the 87235
69	:MEMory:CLEar[:NAME]	Used to clear the frequency response offset table or storage call table specified in the power
69	:MEMory:CLEar:TABLe[1]|2|3|4|5|6|7|8|9|10	Clear the specified frequency response offset table
69	:MEMory:FREE[:ALL]?	Query the total number of bytes unused in the user configuration space and the number of bytes
70	:MEMory:FREE:STATe?	Query the total number of bytes unused in the storage call space and the number of bytes
70	:MEMory:FREE:TABLe?	Query the total number of unused bytes and the number of bytes used in the frequency response offset table
70	:MEMory:NSTates?	Query the number of storage call states, and always return 10
70	:MEMory:STATe:CATalog?	Enumerate the names of all storage call states
70	:MEMory:STATe:DEFine	Query or set the name of the storage call status register.
71	:MEMory:TABLe[1]|2|3|4|5|6|7|8|9|10:DEFine	Query or set the name in the specified frequency response offset table
71	:MEMory:TABLe[1]|2|3|4|5|6|7|8|9|10:FREQuency	Query or set the frequency list in the specified frequency response offset

Index	Command	Brief description of functions
		table
71	:MEMory:TABLe[1]|2|3|4|5|6|7|8|9|10:FREQuency:POINts?	Query the frequency points in the specified frequency response offset table
72	:MEMory:TABLe[1]|2|3|4|5|6|7|8|9|10:GAIN[:MAGNitude]	Query or set the amplitude gain list in the specified frequency response offset table
72	:MEMory:TABLe[1]|2|3|4|5|6|7|8|9|10:GAIN[:MAGNitude]:POINts?	Query the amplitude gain points in the specified frequency response offset table
72	:MEMory:TABLe:MOVE	Rename the specified frequency response offset table
146	:MEMory:TABLe:SELect	Query or set the current frequency response offset table
63	:OUTPut:TRIGger[:STATe]	Query or set the trigger output enable state.
63	:READ[1]|2|3|4[:SCALar][:POWer][:AC]?	Set the specified measurement as absolute power measurement, turn off relative measurement, and return the measured value
64	:READ[1]|2|3|4[:SCALar][:POWer][:AC]:DIFFerence?	Set the specified measurement as differential power measurement, turn off relative measurement, and return the measured value
64	:READ[1]|2|3|4[:SCALar][:POWer][:AC]:DIFFerence:RELative?	Set the specified measurement as differential power measurement, turn on relative measurement, and return the measured value
65	:READ[1]|2|3|4[:SCALar][:POWer][:AC]:RATio?	Set the power measurement mode of the specified measurement as ratio measurement, turn off relative measurement, and return the measured value
65	:READ[1]|2|3|4[:SCALar][:POWer][:AC]:RATio:RELative?	Set the power measurement mode of the specified measurement as ratio measurement, turn on relative measurement, and return the measured value
74	:READ[1]|2|3|4[:SCALar][:POWer][:AC]:RELative?	Set the specified measurement as absolute power measurement, turn on relative measurement, and return the measured value
75	[:SENSe[1]:]AVERage[1]|2:COUNt	Query or set the average number of channel measurements and the average number of videos.
75	[:SENSe[1]:]AVERage:COUNt:AUT	Query or set the channel measurement

Index	Command	Brief description of functions
	O	auto-average state
75	[:SENSe[1]:]AVERage:RESet	Clear the averaging buffer and restart averaging.
75	[:SENSe[1]:]AVERage:SDETect	Query or set the channel step detection state
76	[:SENSe[1]:]AVERage[1]|2[:STATe]	Query or set the channel measurement average and video average switch state
76	[:SENSe[1]:]AVERage[1]|2[:STATe]	Query or set the channel measurement average and video average switch state
77	[:SENSe[1]:]BANDwidth|BWIDth:VIDeo	Query or set the measured video bandwidth.
76	[:SENSe[1]:]BUFFer:COUNt	Query or set the buffer size of external trigger measurement, which is only used for external trigger measurement.
78	[:SENSe[1]:]BUFFer:MTYPe	Query or set the external trigger buffer measurement type, which is only used for external trigger measurement.
78	[:SENSe[1]:]CORRection:CSET2:STATe	Query or set the enable state of the frequency response offset table
78	[:SENSe[1]:]CORRection:DCYCle[:INPut][:MAGNitude]	Query or set the channel duty cycle setting value for pulse power measurement.
79	[:SENSe[1]:]CORRection:DCYCle[:INPut]:STATe	Query or set the channel duty cycle enable switch for pulse power measurement.
79	[:SENSe[1]:]CORRection:FDOFfset[:INPut][:MAGNitude]?	Query the frequency response offset factor.
79	[:SENSe[1]:]CORRection:GAIN[1]|2|3|4[:INPut][:MAGNitude]	Query or set the channel offset
80	[:SENSe[1]:]CORRection:GAIN[1]|2|3|4[:INPut]:STATe	Query or set the channel offset enable state
80	[:SENSe[1]:]DETector:FUNCtion	Query or set the detection measurement method
81	[:SENSe[1]:]FREQuency[:CW|FIXed]	Query or set the frequency.
81	[:SENSe[1]:]FREQuency[:CW|FIXed]:STARt	Query or set the frequency for the start frequency of the external trigger buffer sweep measurement.
82	[:SENSe[1]:]FREQuency[:CW|FIXed]:STEP	Query or set the frequency step number for the external trigger buffer sweep measurement.
83	[:SENSe[1]:]FREQuency[:CW|FIXed]:STOP	Query or set the frequency for the stop frequency of the external trigger buffer sweep measurement.

Index	Command	Brief description of functions
83	[:SENSe[1]:]LIST:FREQuency:STARt	Query or set the start frequency of the timeslot list sweep measurement.
84	[:SENSe[1]:]LIST:FREQuency:STOP	Query or set the stop frequency of the timeslot list sweep measurement.
84	[:SENSe[1]:]LIST:MTYPe	Query or set the timeslot list sweep measurement type, which is only used for external trigger measurement.
85	[:SENSe[1]:]LIST:POINts	Query or set the number of points for timeslot list sweep measurement, which is only used for external trigger measurement.
85	[:SENSe[1]:]LIST:STATe	Query or set the timeslot list sweep measurement state.
85	[:SENSe[1]:]LIST:TSCount	Query or set the number of slots for the timeslot list sweep measurement.
87	[:SENSe[1]:]LIST:SLot:EXCLude:OFFSet:TIME	Query or set the start time (offset time) of the "measurement exclusion area" relative to the start position of the slot.
88	[:SENSe[1]:]LIST:TSLot:EXCLude:TIME	Query or set the time duration of the "measurement exclusion area" relative to the start position of the slot.
88	[:SENSe[1]:]LIST:TSLot:TIME	Query or set the length of time slot measurement.
89	[:SENSe[1]:]LIST:TSLot:TREF[1]|2	Query or set the left and right reference values (percentage relative to the slot duration) of the timeslot measurement gate
89	[:SENSe[1]:]MRATe	Query or set the measurement speed.
90	[:SENSe[1]:]POWer:AC:RANGe	Query or set the current range.
89	[:SENSe[1]:]POWer:AC:RANGe:AUTO	Query or set the automatic range switch state.
91	[:SENSe[1]:]SWEep:APERture	Query or set the measurement aperture or measurement time interval.
91	[:SENSe[1]:]SWEep:APERture:AUTO	Query or set the auto-measurement aperture or measurement interval state.
151	:SERVice:BIST:TBASe:STATe	Query or set the state of the internal 10MHz time base signal output at the "trigger output" port
151	:SERVice:BIST:VIDeo:STATe	Query or set the state of video output signal output at the "trigger output" port
152	:SERVice:SENSor[1]:CDATe?	Query the calibration date of the 87235
152	:SERVice:SENSor[1]:CPLace?	Query the calibration location of the 87235

Index	Command	Brief description of functions
153	:SERVice:SENSor[1]:FREQuency:MAXimum?	Query the maximum frequency of the 87235
153	:SERVice:SENSor[1]:FREQuency:MINimum?	Query the minimum frequency of the 87235
153	:SERVice:SENSor[1]:SNUMber?	Query the serial number of the 87235
153	:SERVice:SENSor[1]:TYPE?	Query the type of the 87235
112	:SERVice:SNUMber	Query or set the serial number of the 87235
112	:STATus:DEVice:CONDition?	Query the value in the device status condition register
112	:STATus:DEVice:ENABle	Query or set the device status event enable register
112	:STATus:DEVice[:EVENt]?	Query the device event register
113	:STATus:DEVice:NTRansition	Query or set the negative transition filter of the device
113	:STATus:DEVice:PTRansition	Query or set the positive transition filter of the device
113	:STATus:OPERation:CALibrating[:SUMMary]:CONDition?	Query the value in the calibration operation status condition register
113	:STATus:OPERation:CALibrating[:SUMMary]:ENABle	Query or set the calibration operation event enable register
114	:STATus:OPERation:CALibrating[:SUMMary][:EVENt]?	Query the calibration operation event register
114	:STATus:OPERation:CALibrating[:SUMMary]:NTRansition	Query or set the negative transition filter for calibration operation
114	:STATus:OPERation:CALibrating[:SUMMary]:PTRansition	Query or set the positive transition filter for calibration operation
115	:STATus:OPERation:CONDition?	Query the value in the operation status condition register
115	:STATus:OPERation:ENABle	Query the value in the operation status condition register
115	:STATus:OPERation[:EVENt]?	Query the operation status event register
115	:STATus:OPERation:LLFail[:SUMMary]:CONDition?	Query the value in the lower limit detection operation status condition register
116	:STATus:OPERation:LLFail[:SUMMary]:ENABle	Query or set the event enable register for lower limit detection operation
116	:STATus:OPERation:LLFail[:SUMMary][:EVENt]?	Query the event register for lower limit detection operation
116	:STATus:OPERation:LLFail[:SUMMary]:NTRansition	Query or set the negative transition filter for lower limit detection operation

Index	Command	Brief description of functions
117	:STATus:OPERation:LLFail[:SUMMary]:PTRansition	Query or set the positive transition filter for lower limit detection operation
117	:STATus:OPERation:NTRansition	Query or set the negative transition filter for operation state
117	:STATus:OPERation:PTRansition	Query or set the positive transition filter for operation state
117	:STATus:OPERation:SENSe[:SUMMary]:CONDition?	Query the value in the sensor operation status condition register
118	:STATus:OPERation:SENSe[:SUMMary]:ENABle	Query or set the sensor operation event enable register
118	:STATus:OPERation:SENSe[:SUMMary][:EVENt]?	Query the event register for sensing operation
118	:STATus:OPERation:SENSe[:SUMMary]:NTRansition	Query or set the negative transition filter for sensing operation
119	:STATus:OPERation:SENSe[:SUMMary]:PTRansition	Query or set the positive transition filter for sensing operation
119	:STATus:OPERation:TRIGger[:SUMMary]:CONDition?	Query the value in the trigger operation status condition register
119	:STATus:OPERation:TRIGger[:SUMMary]:ENABle	Query or set the trigger operation event enable register
119	:STATus:OPERation:TRIGger[:SUMMary][:EVENt]?	Query the event register for trigger operation
120	:STATus:OPERation:TRIGger[:SUMMary]:NTRansition	Query or set the negative transition filter for trigger operation
120	:STATus:OPERation:TRIGger[:SUMMary]:PTRansition	Query or set the positive transition filter for trigger operation
120	:STATus:OPERation:ULFail[:SUMMary]:CONDition?	Query the value in the upper limit detection operation status condition register
121	:STATus:OPERation:ULFail[:SUMMary]:ENABle	Query or set the event enable register for upper limit detection operation
121	:STATus:OPERation:ULFail[:SUMMary][:EVENt]?	Query the event register for upper limit detection operation
121	:STATus:OPERation:ULFail[:SUMMary]:NTRansition	Query or set the negative transition filter for upper limit detection operation
122	:STATus:OPERation:ULFail[:SUMMary]:PTRansition	Query or set the positive transition filter for upper limit detection operation
122	:STATus:PRESet	Preset some state registers
122	:STATus:QUEStionable:CALibration[:SUMMary]:CONDition?	Query the value in the calibration questionable status condition register
123	:STATus:QUEStionable:CALibration[:SUMMary]:ENABle	Query or set the calibration questionable event enable register

Index	Command	Brief description of functions
123	:STATus:QUEStionable:CALibration[:SUMMary][:EVENt]?	Query the calibration operation event register
123	:STATus:QUEStionable:CALibration[:SUMMary]:NTRansition	Query or set the questionable negative transition filter for calibration operation
123	:STATus:QUEStionable:CALibration[:SUMMary]:PTRansition	Query or set the questionable positive transition filter for calibration operation
124	:STATus:QUEStionable:CONDition?	Query the value in the questionable status condition register
124	:STATus:QUEStionable:ENABle	Query or set the questionable status event enable register
124	:STATus:QUEStionable[:EVENt]?	Query the questionable status event register
125	:STATus:QUEStionable:NTRansition	Query or set the questionable negative transition filter for operation state
125	:STATus:QUEStionable:POWer[:SUMMary]:CONDition?	Query the value in the power questionable status condition register
125	:STATus:QUEStionable:POWer[:SUMMary]:ENABle	Query or set the power questionable event enable register
126	:STATus:QUEStionable:POWer[:SUMMary][:EVENt]?	Query the questionable event register for power operation
126	:STATus:QUEStionable:POWer[:SUMMary]:NTRansition	Query or set the questionable negative transition filter for power operation
126	:STATus:QUEStionable:POWer[:SUMMary]:PTRansition	Query or set the questionable positive transition filter for power operation
128	:STATus:QUEStionable:PTRansition	Query or set the questionable positive transition filter for operation state
128	:SYSTem:ERRor:CODE?	Return error code from error queue
128	:SYSTem:ERRor[:NEXT]?	Return error code and error information from the error queue
129	:SYSTem:HELP:HEADers?	Query the list of commands supported by 87235
129	:SYSTem:IDN	Query or set "*IDN?" of the 87235 Query the returned user-defined string.
129	:SYSTem:IDN:AUTO	Query or set the "*IDN?" of the 87235 Whether to return the switch of the user-defined string.
130	:SYSTem:PRESet	Reset 87235 to the state specified by the parameter
142	:SYSTem:VERSion?	Query the SCPI version number used by 87235
146	:TRIGger[1][:IMMediate]	Set to be in Wait for Trigger state
147	:TRIGger:MODE	Query or set the trigger mode of the 87235

Index	Command	Brief description of functions
147	:TRIGger[:SEQuence[1]]:COUNt	Query or set the number of trigger event detection/measurement cycles.
148	:TRIGger[:SEQuence[1]]:DELay	Query or set the trigger delay
148	:TRIGger[:SEQuence[1]]:HOLDoff	Query or set the trigger holdoff
148	:TRIGger[:SEQuence[1]]:IMMediate	Set to be in Wait for Trigger state
148	:TRIGger[:SEQuence[1]]:POSition	Query or set the position of the trigger event on the screen
149	:TRIGger[:SEQuence[1]]:SLOPe	Query or set the trigger type
149	:TRIGger[:SEQuence[1]]:SOURce	Query or set the trigger source.
150	:UNIT[1]|2|3|4:POWer	Query or set the unit of measured power
150	:UNIT[1]|2|3|4:POWer:RATio	Query or set the unit of measured ratio measurement power